

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031889.D
 Acq On : 10 May 2019 15:26
 Operator : JC/SP
 Sample : K2742-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB4	15289	14964	0.10%	0.028%
2	1.396	88	95	107	rBV	582569	612418	3.90%	1.161%
3	1.672	173	181	199	rVB	432489	584512	3.72%	1.108%
4	2.267	355	366	376	rBV	921068	1402242	8.92%	2.658%
5	2.318	376	382	405	rVB	101572	176106	1.12%	0.334%
6	2.444	413	421	437	rVB	41449	73993	0.47%	0.140%
7	2.650	482	485	487	rBV2	1246	731	0.00%	0.001%
8	2.688	495	497	499	rBV3	1073	645	0.00%	0.001%
9	2.749	512	516	519	rBV4	1135	866	0.01%	0.002%
10	2.833	525	542	567	rBV	327890	721913	4.59%	1.369%
11	2.990	587	591	592	rBV3	1515	1051	0.01%	0.002%
12	3.058	610	612	618	rBV5	580	544	0.00%	0.001%
13	3.154	639	642	645	rVB3	1023	685	0.00%	0.001%
14	3.180	645	650	654	rBV5	1325	1431	0.01%	0.003%
15	3.286	679	683	686	rBV3	839	655	0.00%	0.001%
16	3.306	686	689	694	rVV5	1006	933	0.01%	0.002%
17	3.363	703	707	709	rBV3	928	641	0.00%	0.001%
18	3.415	720	723	728	rVB5	799	596	0.00%	0.001%
19	3.553	763	766	768	rVV	823	595	0.00%	0.001%
20	3.566	768	770	775	rVV3	937	664	0.00%	0.001%
21	3.601	776	781	785	rVV4	903	1023	0.01%	0.002%
22	3.685	804	807	813	rVB5	563	528	0.00%	0.001%
23	3.759	823	830	831	rBV5	597	639	0.00%	0.001%
24	3.887	868	870	873	rBV2	822	483	0.00%	0.001%
25	3.939	884	886	889	rVB3	817	433	0.00%	0.001%
26	3.955	889	891	893	rBV2	739	430	0.00%	0.001%
27	4.019	907	911	913	rBV	678	535	0.00%	0.001%
28	4.042	913	918	921	rBV3	630	422	0.00%	0.001%
29	4.119	935	942	944	rBV5	1851	2200	0.01%	0.004%
30	4.174	944	959	1005	rBV2	487139	1550272	9.87%	2.939%
31	4.643	1088	1105	1131	rBV	685502	1635489	10.41%	3.100%
32	4.797	1150	1153	1160	rBV4	2187	1885	0.01%	0.004%
33	4.862	1170	1173	1176	rBV3	2457	1899	0.01%	0.004%
34	5.125	1253	1255	1258	rVV3	847	586	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031889.D
 Acq On : 10 May 2019 15:26
 Operator : JC/SP
 Sample : K2742-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.183	1268	1273	1277	rBV6	1079	1081	0.01%	0.002%
36	5.334	1293	1320	1358	rBV2	1424044	4354658	27.72%	8.255%
37	5.881	1477	1490	1514	rBV	1221772	2493671	15.87%	4.727%
38	6.325	1615	1628	1656	rBV	949356	1932335	12.30%	3.663%
39	6.759	1761	1763	1767	rVV3	1482	894	0.01%	0.002%
40	6.788	1770	1772	1775	rVB2	960	425	0.00%	0.001%
41	6.817	1775	1781	1784	rBV4	1266	1373	0.01%	0.003%
42	6.862	1792	1795	1798	rBV4	1921	1469	0.01%	0.003%
43	7.019	1840	1844	1848	rBV5	1220	1063	0.01%	0.002%
44	7.161	1886	1888	1892	rVB2	958	462	0.00%	0.001%
45	7.225	1896	1908	1928	rBV	490447	887825	5.65%	1.683%
46	7.563	1999	2013	2060	rBV	1724344	3283841	20.90%	6.225%
47	7.846	2091	2101	2122	rBV	326785	586201	3.73%	1.111%
48	8.100	2177	2180	2182	rBV4	1239	690	0.00%	0.001%
49	8.173	2192	2203	2214	rBV2	44346	78409	0.50%	0.149%
50	8.260	2228	2230	2233	rVB2	1083	622	0.00%	0.001%
51	8.309	2233	2245	2295	rBV	1282135	2455043	15.63%	4.654%
52	8.743	2377	2380	2382	rBV4	1857	1193	0.01%	0.002%
53	8.958	2444	2447	2450	rBV4	1183	760	0.00%	0.001%
54	9.013	2461	2464	2468	rBV2	978	803	0.01%	0.002%
55	9.087	2472	2487	2493	rBV	1913537	3367111	21.43%	6.383%
56	9.440	2594	2597	2600	rBV3	1944	1355	0.01%	0.003%
57	9.646	2658	2661	2662	rBV2	1017	578	0.00%	0.001%
58	9.662	2664	2666	2669	rVB3	1714	882	0.01%	0.002%
59	9.681	2669	2672	2673	rBV3	760	422	0.00%	0.001%
60	9.749	2690	2693	2694	rBV	959	572	0.00%	0.001%
61	9.765	2695	2698	2699	rVV3	1387	893	0.01%	0.002%
62	9.784	2702	2704	2707	rVB	1695	930	0.01%	0.002%
63	9.961	2756	2759	2760	rBV2	1338	630	0.00%	0.001%
64	10.054	2784	2788	2792	rBV5	1642	1552	0.01%	0.003%
65	10.077	2792	2795	2797	rBV3	1437	852	0.01%	0.002%
66	10.112	2804	2806	2810	rVB4	832	466	0.00%	0.001%
67	10.199	2831	2833	2836	rVB3	1088	546	0.00%	0.001%
68	10.218	2836	2839	2841	rBV2	919	471	0.00%	0.001%
69	10.251	2847	2849	2853	rVB2	947	466	0.00%	0.001%
70	10.296	2860	2863	2865	rBV2	999	551	0.00%	0.001%
71	10.321	2869	2871	2877	rVB5	1286	900	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031889.D
 Acq On : 10 May 2019 15:26
 Operator : JC/SP
 Sample : K2742-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2926	rBV	1300160	2126073	13.53%	4.030%
73	10.604	2949	2959	2973	rVB2	42693	72228	0.46%	0.137%
74	10.659	2973	2976	2977	rBV2	1020	566	0.00%	0.001%
75	10.752	3000	3005	3006	rBV4	1122	990	0.01%	0.002%
76	10.807	3020	3022	3025	rVV2	1017	603	0.00%	0.001%
77	10.852	3032	3036	3039	rBV3	1046	897	0.01%	0.002%
78	10.900	3049	3051	3057	rBV4	991	835	0.01%	0.002%
79	11.029	3089	3091	3094	rVB3	946	463	0.00%	0.001%
80	11.080	3103	3107	3110	rBV4	2020	1865	0.01%	0.004%
81	11.148	3125	3128	3130	rBV3	703	451	0.00%	0.001%
82	11.199	3141	3144	3147	rVV3	1298	913	0.01%	0.002%
83	11.357	3190	3193	3195	rBV2	1332	792	0.01%	0.002%
84	11.415	3197	3211	3220	rBV	174096	292592	1.86%	0.555%
85	11.482	3220	3232	3236	rBV	1850047	3070913	19.55%	5.822%
86	11.765	3312	3320	3328	rBV6	8678	17166	0.11%	0.033%
87	11.874	3336	3354	3385	rBV3	8420565	15711687	100.00%	29.785%
88	12.476	3531	3541	3556	rVB	20758	36360	0.23%	0.069%
89	12.601	3577	3580	3581	rBV	1305	740	0.00%	0.001%
90	12.640	3581	3592	3604	rVV	7833	15691	0.10%	0.030%
91	12.861	3650	3661	3678	rBV2	181642	361868	2.30%	0.686%
92	13.286	3790	3793	3796	rBV5	1926	1361	0.01%	0.003%
93	13.360	3812	3816	3820	rBV4	2123	1974	0.01%	0.004%
94	13.498	3847	3859	3883	rBV	1477513	2421240	15.41%	4.590%
95	13.832	3960	3963	3966	rBV4	1866	1468	0.01%	0.003%
96	13.984	3997	4010	4031	rBV	1163374	1942218	12.36%	3.682%
97	14.276	4094	4101	4108	rVB3	8516	12251	0.08%	0.023%
98	14.402	4129	4140	4154	rBV7	29347	83313	0.53%	0.158%
99	15.074	4344	4349	4364	rVB5	20197	34762	0.22%	0.066%
100	15.649	4518	4528	4551	rBV3	137506	282434	1.80%	0.535%


Sum of corrected areas: 52749718

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051019\
Data File : VU031889.D
Acq On : 10 May 2019 15:26
Operator : JC/SP
Sample : K2742-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

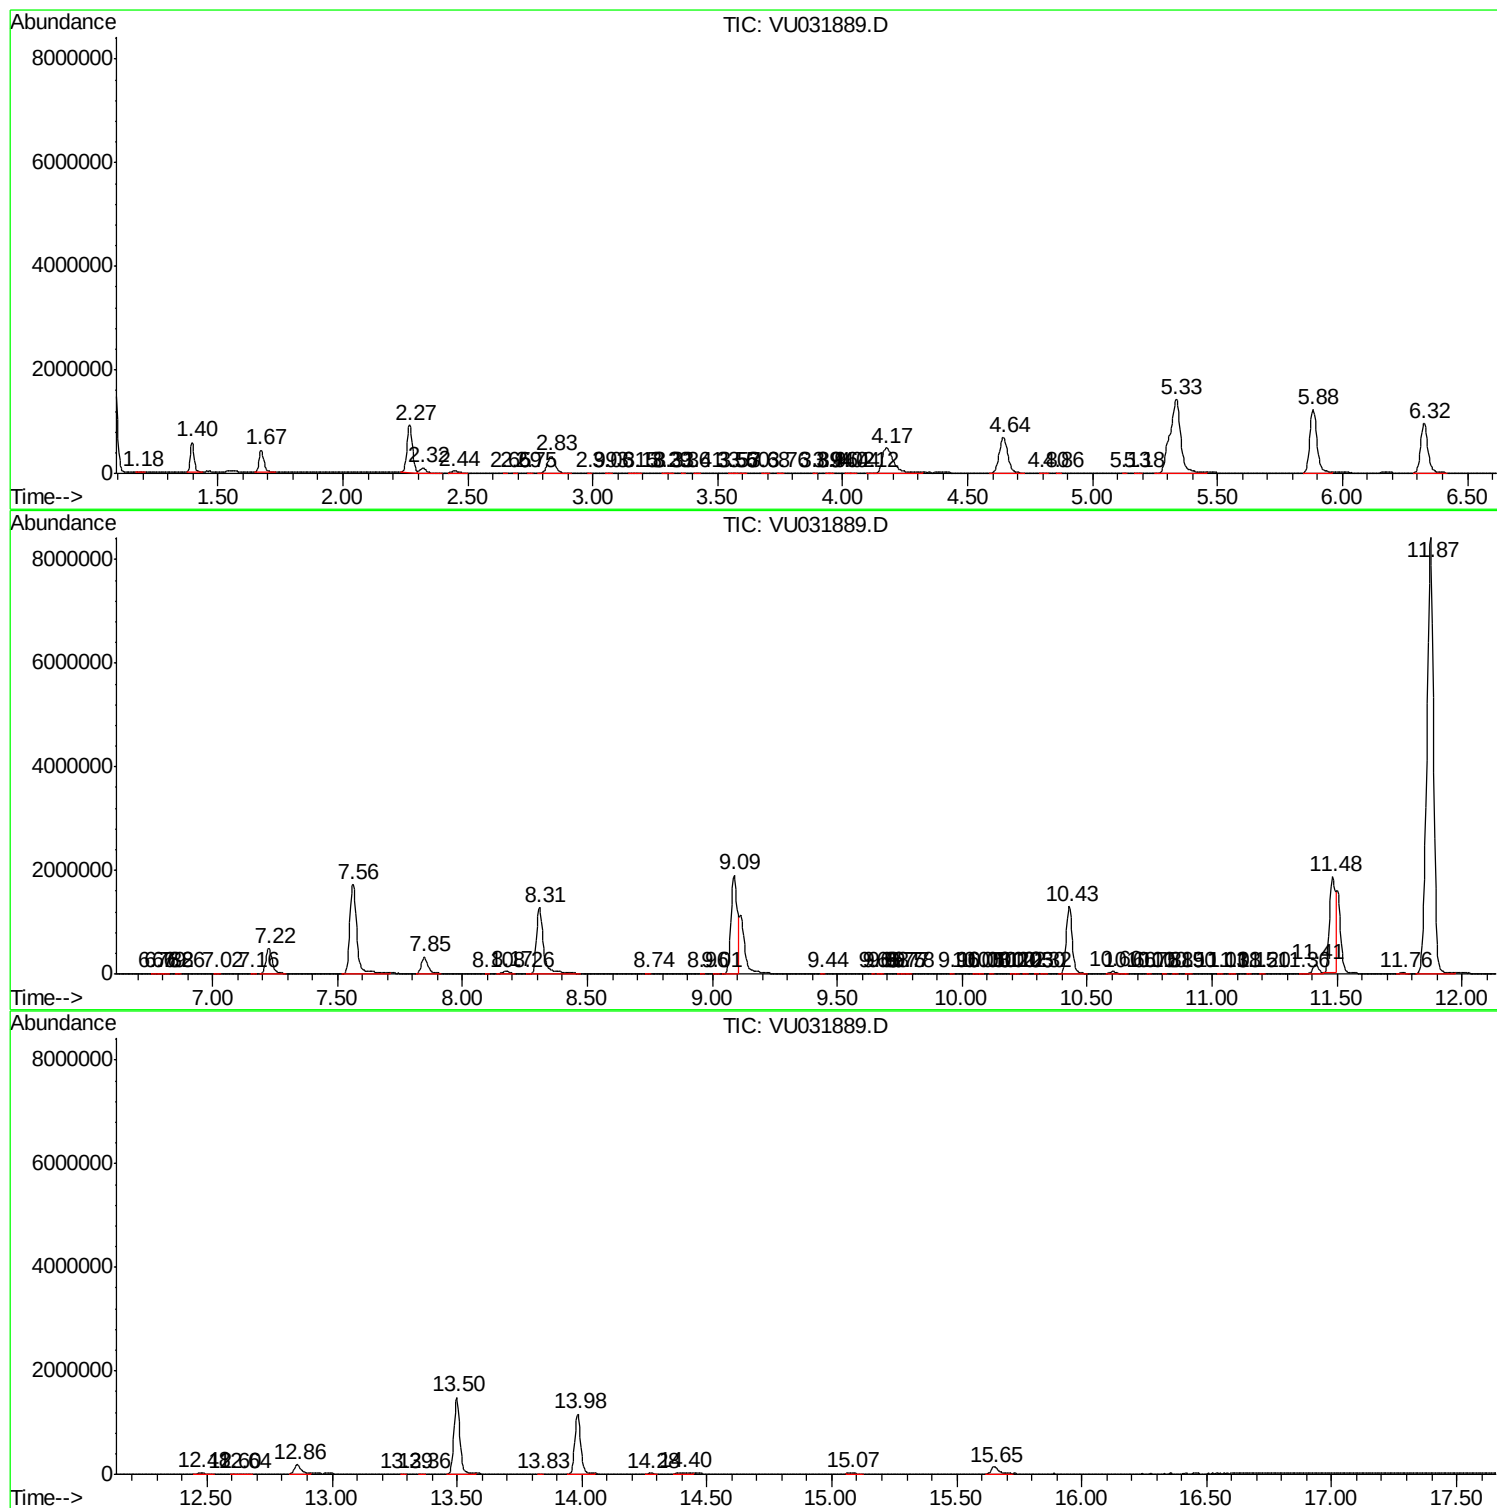

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031889.D
Acq On : 10 May 2019 15:26
Operator : JC/SP
Sample : K2742-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031889.D
Acq On : 10 May 2019 15:26
Operator : JC/SP
Sample : K2742-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc