

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031905.D
 Acq On : 10 May 2019 21:54
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	39	rVB2	17612	18448	0.42%	0.056%
2	1.395	88	95	106	rBV	632717	661845	14.91%	2.023%
3	1.669	172	180	199	rVB	468598	625355	14.09%	1.911%
4	2.267	355	366	379	rVB	973016	1483251	33.41%	4.534%
5	2.547	450	453	455	rBV3	1197	789	0.02%	0.002%
6	2.598	465	469	472	rBV3	1253	1246	0.03%	0.004%
7	2.698	493	500	506	rVB5	4170	5195	0.12%	0.016%
8	2.756	513	518	522	rBV5	1621	1311	0.03%	0.004%
9	2.813	532	536	537	rBV3	868	599	0.01%	0.002%
10	2.833	539	542	546	rVV2	2025	1832	0.04%	0.006%
11	2.852	546	548	551	rVV2	968	661	0.01%	0.002%
12	2.923	564	570	573	rVB6	1069	1131	0.03%	0.003%
13	3.003	592	595	597	rBV3	842	594	0.01%	0.002%
14	3.016	597	599	605	rVV4	942	839	0.02%	0.003%
15	3.161	642	644	649	rVB3	895	620	0.01%	0.002%
16	3.186	649	652	657	rVB6	1046	793	0.02%	0.002%
17	3.293	681	685	689	rBV5	897	946	0.02%	0.003%
18	3.386	709	714	719	rBV3	1834	2078	0.05%	0.006%
19	3.463	732	738	740	rBV2	1232	1149	0.03%	0.004%
20	3.575	769	773	778	rBV4	807	729	0.02%	0.002%
21	3.624	783	788	792	rVB2	632	541	0.01%	0.002%
22	3.720	813	818	823	rVB5	1299	1606	0.04%	0.005%
23	3.820	844	849	853	rBV4	662	755	0.02%	0.002%
24	3.942	884	887	891	rVB2	763	653	0.01%	0.002%
25	4.000	901	905	908	rBV2	738	577	0.01%	0.002%
26	4.016	908	910	919	rVB3	1354	1173	0.03%	0.004%
27	4.058	919	923	925	rBV	934	628	0.01%	0.002%
28	4.071	925	927	931	rVB2	1319	851	0.02%	0.003%
29	4.170	946	958	992	rBV	413644	1109867	25.00%	3.392%
30	4.553	1075	1077	1081	rVB3	1449	837	0.02%	0.003%
31	4.640	1085	1104	1130	rBV	713405	1705885	38.42%	5.214%
32	4.845	1165	1168	1171	rBV3	1520	1198	0.03%	0.004%
33	5.080	1238	1241	1243	rBV2	724	483	0.01%	0.001%
34	5.209	1277	1281	1285	rBV4	1113	983	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U051019\
 Data File : VU031905.D
 Acq On : 10 May 2019 21:54
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1293	1320	1362	rBV2	1481867	4439550	100.00%	13.569%
36	5.881	1476	1490	1520	rBV	1240434	2533511	57.07%	7.744%
37	6.177	1572	1582	1601	rVB7	14143	32872	0.74%	0.100%
38	6.325	1614	1628	1651	rBV	993232	1996758	44.98%	6.103%
39	6.656	1729	1731	1738	rVB5	1503	1331	0.03%	0.004%
40	6.697	1742	1744	1747	rVB4	960	467	0.01%	0.001%
41	6.717	1747	1750	1753	rVB3	870	510	0.01%	0.002%
42	6.733	1753	1755	1757	rBV2	1063	564	0.01%	0.002%
43	6.874	1797	1799	1803	rVV3	758	463	0.01%	0.001%
44	6.900	1803	1807	1811	rVV4	867	700	0.02%	0.002%
45	6.923	1811	1814	1818	rVB3	996	721	0.02%	0.002%
46	6.952	1818	1823	1828	rBV5	1309	1362	0.03%	0.004%
47	6.993	1833	1836	1840	rVV4	708	677	0.02%	0.002%
48	7.048	1844	1853	1857	rVB6	1347	1877	0.04%	0.006%
49	7.080	1859	1863	1866	rBV3	1212	924	0.02%	0.003%
50	7.135	1875	1880	1883	rBV3	850	634	0.01%	0.002%
51	7.225	1893	1908	1928	rBV	491387	903872	20.36%	2.763%
52	7.476	1983	1986	1991	rBV5	1240	885	0.02%	0.003%
53	7.505	1992	1995	1998	rBV3	964	694	0.02%	0.002%
54	7.562	1998	2013	2058	rBV	1773705	3349481	75.45%	10.238%
55	7.845	2091	2101	2116	rBV	338744	592888	13.35%	1.812%
56	8.064	2167	2169	2171	rBV3	1329	826	0.02%	0.003%
57	8.096	2176	2179	2184	rBV5	981	886	0.02%	0.003%
58	8.308	2233	2245	2289	rBV	1308191	2528029	56.94%	7.727%
59	8.691	2362	2364	2367	rBV4	1226	701	0.02%	0.002%
60	8.842	2409	2411	2416	rVB4	1518	1140	0.03%	0.003%
61	8.961	2440	2448	2452	rBV9	1715	2007	0.05%	0.006%
62	9.006	2460	2462	2464	rBV2	1024	551	0.01%	0.002%
63	9.022	2464	2467	2472	rVB2	1433	984	0.02%	0.003%
64	9.086	2474	2487	2532	rBV	1827611	3284641	73.99%	10.039%
65	9.672	2666	2669	2672	rBV4	1636	1164	0.03%	0.004%
66	9.697	2672	2677	2679	rVV4	977	778	0.02%	0.002%
67	9.771	2696	2700	2704	rBV4	1347	1157	0.03%	0.004%
68	9.942	2750	2753	2756	rBV3	884	585	0.01%	0.002%
69	9.961	2756	2759	2762	rVV3	1446	876	0.02%	0.003%
70	9.987	2764	2767	2770	rVB2	1159	765	0.02%	0.002%
71	10.103	2800	2803	2806	rBV3	804	628	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031905.D
 Acq On : 10 May 2019 21:54
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.144	2812	2816	2819	rBV3	1199	914	0.02%	0.003%
73	10.218	2835	2839	2843	rBV4	1356	1128	0.03%	0.003%
74	10.427	2891	2904	2929	rBV	1328694	2149013	48.41%	6.568%
75	10.598	2955	2957	2962	rVB5	1874	1453	0.03%	0.004%
76	10.649	2971	2973	2976	rVB4	1063	532	0.01%	0.002%
77	10.826	3025	3028	3030	rBV3	1034	607	0.01%	0.002%
78	10.855	3035	3037	3040	rVV3	728	466	0.01%	0.001%
79	11.048	3095	3097	3100	rVB	1110	576	0.01%	0.002%
80	11.080	3104	3107	3116	rVB7	2267	2746	0.06%	0.008%
81	11.115	3116	3118	3121	rBV4	975	669	0.02%	0.002%
82	11.170	3130	3135	3137	rBV3	740	648	0.01%	0.002%
83	11.186	3137	3140	3146	rVV4	1279	895	0.02%	0.003%
84	11.218	3146	3150	3154	rBV4	763	737	0.02%	0.002%
85	11.276	3164	3168	3172	rBV3	1534	1293	0.03%	0.004%
86	11.305	3172	3177	3178	rBV2	1089	892	0.02%	0.003%
87	11.360	3191	3194	3196	rVV2	961	607	0.01%	0.002%
88	11.424	3208	3214	3220	rBV6	2768	3775	0.09%	0.012%
89	11.482	3220	3232	3254	rBV	1472337	2493811	56.17%	7.622%
90	11.855	3335	3348	3373	rBV	1594748	2723363	61.34%	8.324%
91	12.479	3539	3542	3546	rVB5	2199	1619	0.04%	0.005%
92	12.575	3570	3572	3574	rBV2	1256	643	0.01%	0.002%
93	12.717	3613	3616	3618	rBV	1091	645	0.01%	0.002%
94	12.903	3672	3674	3679	rBV5	1150	648	0.01%	0.002%
95	13.003	3699	3705	3708	rBV3	2640	2760	0.06%	0.008%
96	13.376	3818	3821	3822	rBV2	1133	632	0.01%	0.002%
97	13.527	3865	3868	3870	rBV3	1612	1273	0.03%	0.004%
98	13.684	3915	3917	3920	rBV3	1510	708	0.02%	0.002%
99	14.704	4231	4234	4236	rBV3	1544	987	0.02%	0.003%
100	14.781	4255	4258	4261	rBV4	1866	1274	0.03%	0.004%


Sum of corrected areas: 32717221

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051019\
Data File : VU031905.D
Acq On : 10 May 2019 21:54
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

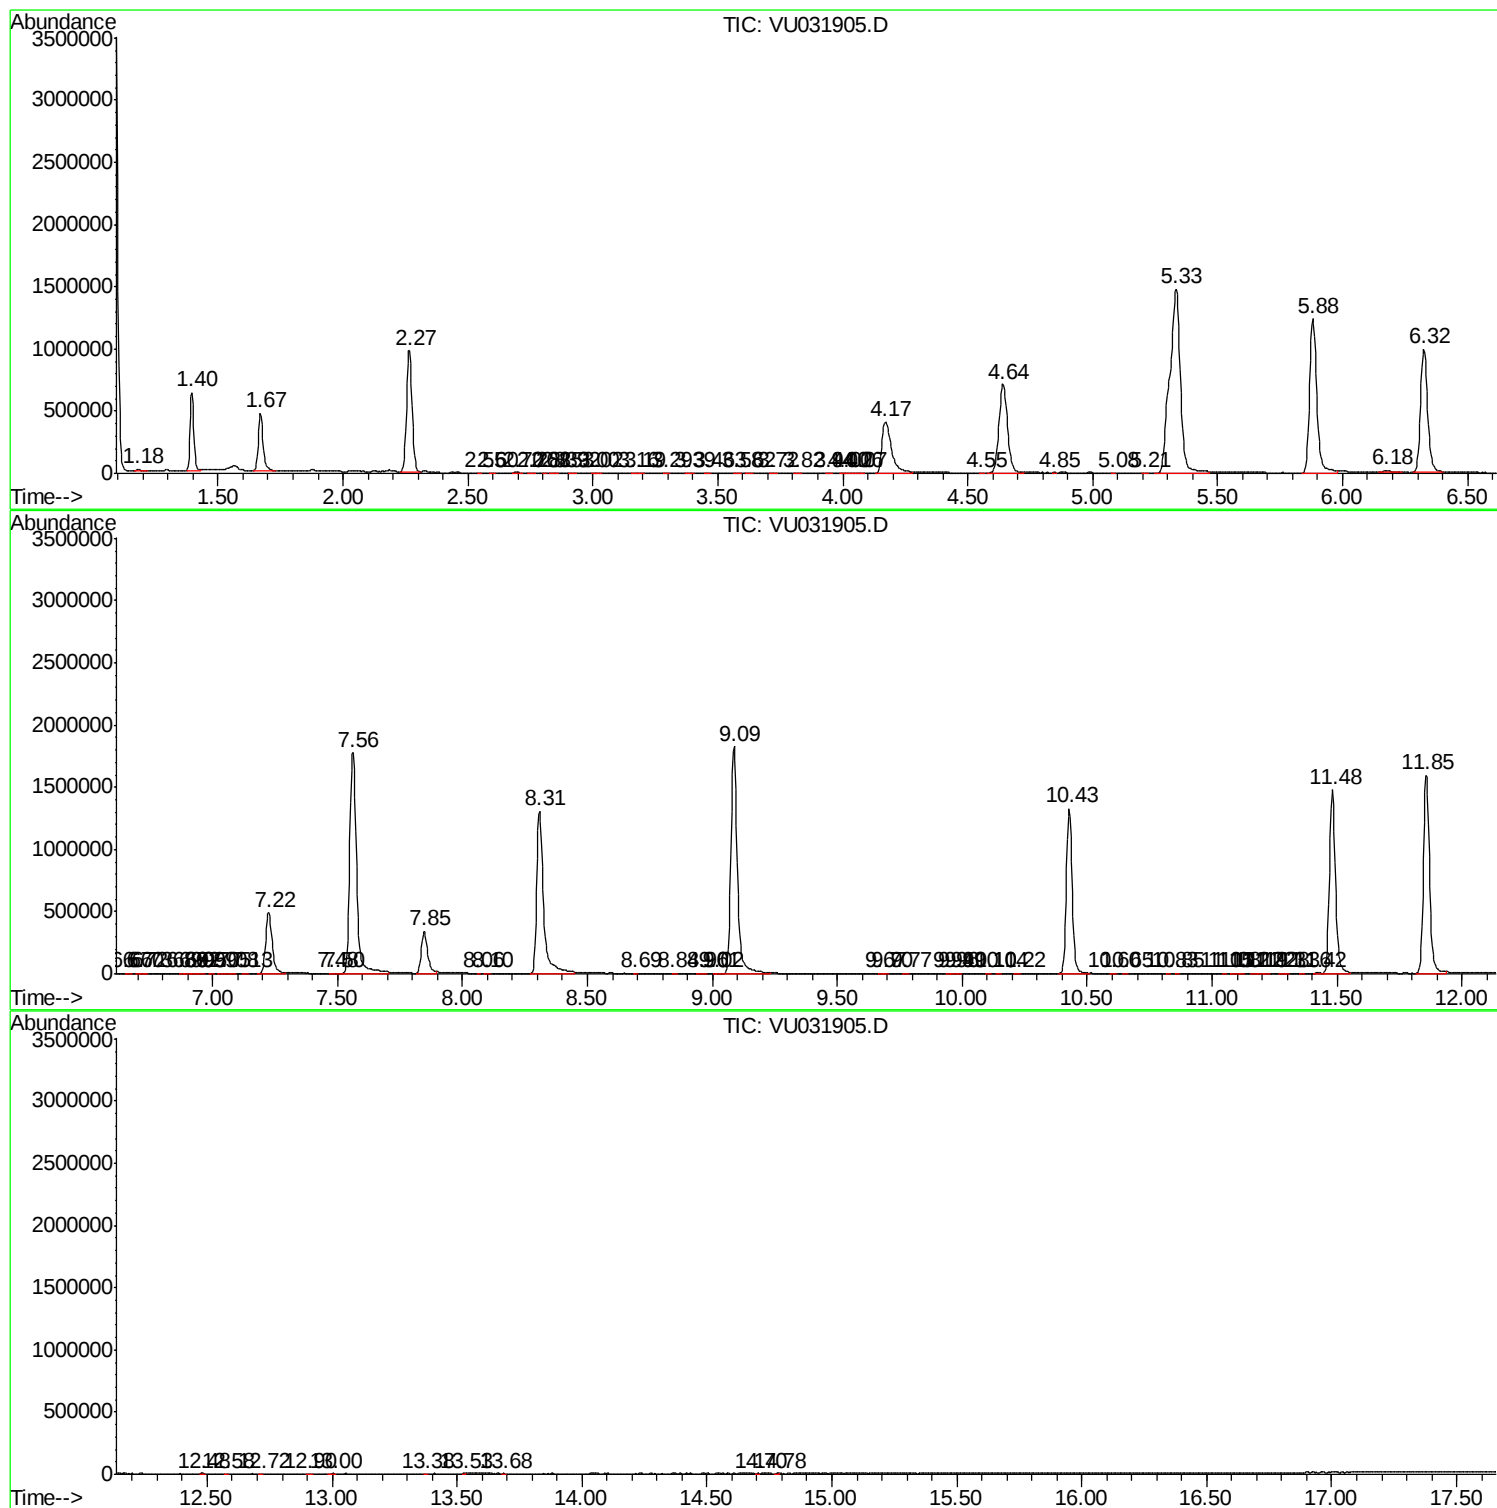

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031905.D
Acq On : 10 May 2019 21:54
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031905.D
Acq On : 10 May 2019 21:54
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
