

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031910.D
 Acq On : 10 May 2019 23:53
 Operator : JC/SP
 Sample : K2705-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	35	rVB3	16725	12766	0.31%	0.038%
2	1.395	88	95	107	rBV	604199	624156	14.96%	1.859%
3	1.669	172	180	200	rVB	423060	574991	13.78%	1.713%
4	2.267	355	366	378	rBV	870886	1334567	31.98%	3.975%
5	2.447	413	422	442	rVB	41368	76420	1.83%	0.228%
6	2.659	485	488	492	rVB4	1225	805	0.02%	0.002%
7	2.694	492	499	502	rBV5	2097	2484	0.06%	0.007%
8	2.762	511	520	521	rBV4	1689	2138	0.05%	0.006%
9	2.833	529	542	558	rVB	53654	114007	2.73%	0.340%
10	2.907	563	565	569	rVB4	774	593	0.01%	0.002%
11	2.987	579	590	591	rBV7	12119	16282	0.39%	0.048%
12	3.045	605	608	614	rVB5	912	729	0.02%	0.002%
13	3.103	620	626	628	rBV4	976	920	0.02%	0.003%
14	3.264	672	676	679	rBV	2006	1713	0.04%	0.005%
15	3.382	711	713	718	rVV3	1099	955	0.02%	0.003%
16	3.447	729	733	734	rBV4	824	651	0.02%	0.002%
17	3.482	741	744	746	rBV2	1017	736	0.02%	0.002%
18	3.514	751	754	762	rBV4	907	1219	0.03%	0.004%
19	3.585	772	776	781	rVB4	1374	1267	0.03%	0.004%
20	3.640	787	793	798	rBV3	1231	1149	0.03%	0.003%
21	3.752	821	828	834	rBV5	789	1119	0.03%	0.003%
22	3.855	856	860	865	rVB3	862	996	0.02%	0.003%
23	4.103	932	937	939	rBV2	946	817	0.02%	0.002%
24	4.173	945	959	964	rBV	426008	886691	21.25%	2.641%
25	4.489	1053	1057	1061	rVB6	2039	2136	0.05%	0.006%
26	4.517	1061	1066	1071	rBV7	2350	2839	0.07%	0.008%
27	4.643	1089	1105	1131	rBV	668359	1575088	37.75%	4.692%
28	4.845	1166	1168	1172	rVB4	1469	750	0.02%	0.002%
29	5.135	1253	1258	1261	rVB4	1962	1535	0.04%	0.005%
30	5.196	1274	1277	1280	rVB5	903	659	0.02%	0.002%
31	5.244	1285	1292	1294	rBV7	1087	1207	0.03%	0.004%
32	5.334	1294	1320	1358	rBV2	1374445	4172647	100.00%	12.429%
33	5.742	1444	1447	1448	rBV3	1008	589	0.01%	0.002%
34	5.810	1464	1468	1472	rVB5	1564	1429	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U051019\
 Data File : VU031910.D
 Acq On : 10 May 2019 23:53
 Operator : JC/SP
 Sample : K2705-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1476	1490	1516	rBV	1173001	2408937	57.73%	7.175%
36	6.180	1569	1583	1615	rBV	1374559	2764483	66.25%	8.234%
37	6.324	1616	1628	1658	rVB	927212	1904289	45.64%	5.672%
38	6.710	1746	1748	1755	rVB4	1438	1371	0.03%	0.004%
39	6.762	1761	1764	1768	rBV2	1108	855	0.02%	0.003%
40	6.810	1775	1779	1782	rVB2	945	698	0.02%	0.002%
41	6.832	1782	1786	1788	rBV3	1637	1051	0.03%	0.003%
42	6.871	1794	1798	1800	rBV4	960	816	0.02%	0.002%
43	7.000	1834	1838	1840	rBV4	1072	926	0.02%	0.003%
44	7.045	1850	1852	1856	rVB3	1001	592	0.01%	0.002%
45	7.225	1894	1908	1938	rBV	468687	866706	20.77%	2.582%
46	7.562	1998	2013	2033	rBV	1669811	3010426	72.15%	8.967%
47	7.845	2091	2101	2128	rBV	312524	570090	13.66%	1.698%
48	8.000	2147	2149	2154	rBV5	1449	1010	0.02%	0.003%
49	8.115	2182	2185	2191	rVB5	1689	1495	0.04%	0.004%
50	8.151	2191	2196	2197	rBV2	1046	906	0.02%	0.003%
51	8.173	2197	2203	2209	rBV6	4216	6012	0.14%	0.018%
52	8.225	2209	2219	2234	rVV2	82693	146565	3.51%	0.437%
53	8.308	2234	2245	2291	rBV	1266945	2470033	59.20%	7.357%
54	8.717	2370	2372	2380	rVB6	2231	1926	0.05%	0.006%
55	8.797	2395	2397	2402	rVB4	1122	879	0.02%	0.003%
56	8.823	2402	2405	2407	rBV3	1226	860	0.02%	0.003%
57	8.897	2426	2428	2431	rBV2	1289	616	0.01%	0.002%
58	8.913	2431	2433	2436	rVV3	1196	654	0.02%	0.002%
59	9.086	2473	2487	2539	rBV	1740136	3099865	74.29%	9.233%
60	9.447	2592	2599	2602	rBV6	2128	2591	0.06%	0.008%
61	9.495	2611	2614	2618	rBV3	1219	913	0.02%	0.003%
62	9.559	2631	2634	2637	rBV2	1235	877	0.02%	0.003%
63	9.691	2672	2675	2679	rVB4	1224	884	0.02%	0.003%
64	9.717	2680	2683	2689	rVB5	1336	985	0.02%	0.003%
65	9.794	2701	2707	2708	rBV5	1531	1158	0.03%	0.003%
66	9.861	2724	2728	2731	rBV3	692	550	0.01%	0.002%
67	9.971	2760	2762	2767	rVV4	879	676	0.02%	0.002%
68	10.003	2767	2772	2779	rVB6	1324	1926	0.05%	0.006%
69	10.038	2779	2783	2788	rVB4	962	825	0.02%	0.002%
70	10.067	2788	2792	2796	rBV4	1444	1694	0.04%	0.005%
71	10.167	2819	2823	2826	rVB3	1089	810	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051019\
 Data File : VU031910.D
 Acq On : 10 May 2019 23:53
 Operator : JC/SP
 Sample : K2705-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.266	2850	2854	2857	rBV2	796	597	0.01%	0.002%
73	10.353	2878	2881	2885	rBV2	784	577	0.01%	0.002%
74	10.427	2891	2904	2931	rBV	1306645	2113457	50.65%	6.295%
75	10.598	2953	2957	2958	rBV4	2550	1820	0.04%	0.005%
76	10.864	3036	3040	3043	rBV3	1099	771	0.02%	0.002%
77	10.897	3047	3050	3056	rVB5	1741	1235	0.03%	0.004%
78	11.189	3138	3141	3146	rVB3	1721	1497	0.04%	0.004%
79	11.215	3146	3149	3151	rBV3	871	592	0.01%	0.002%
80	11.324	3177	3183	3187	rBV4	990	1096	0.03%	0.003%
81	11.398	3202	3206	3207	rBV4	1388	1021	0.02%	0.003%
82	11.479	3219	3231	3258	rBV	1385687	2291514	54.92%	6.825%
83	11.855	3336	3348	3373	rBV	1441757	2449434	58.70%	7.296%
84	12.372	3506	3509	3512	rBV3	1364	779	0.02%	0.002%
85	12.395	3512	3516	3519	rBV4	1641	1450	0.03%	0.004%
86	12.466	3535	3538	3541	rBV3	2538	2426	0.06%	0.007%
87	12.594	3576	3578	3580	rBV2	1220	651	0.02%	0.002%
88	12.652	3593	3596	3598	rVB3	1116	672	0.02%	0.002%
89	12.778	3632	3635	3638	rBV3	1449	1023	0.02%	0.003%
90	12.932	3680	3683	3685	rBV3	1281	744	0.02%	0.002%
91	12.961	3689	3692	3694	rBV	1044	728	0.02%	0.002%
92	13.057	3719	3722	3725	rBV2	1537	962	0.02%	0.003%
93	13.253	3781	3783	3788	rVB2	1261	749	0.02%	0.002%
94	13.462	3845	3848	3853	rBV5	1387	1268	0.03%	0.004%
95	13.716	3924	3927	3931	rBV4	1167	1022	0.02%	0.003%
96	14.025	4021	4023	4025	rBV3	1074	555	0.01%	0.002%
97	14.215	4078	4082	4084	rBV4	1309	936	0.02%	0.003%
98	14.289	4103	4105	4108	rBV4	1627	969	0.02%	0.003%
99	14.443	4151	4153	4157	rBV4	1077	858	0.02%	0.003%
100	14.588	4196	4198	4200	rBV2	947	579	0.01%	0.002%


Sum of corrected areas: 33572982

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051019\
Data File : VU031910.D
Acq On : 10 May 2019 23:53
Operator : JC/SP
Sample : K2705-13
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

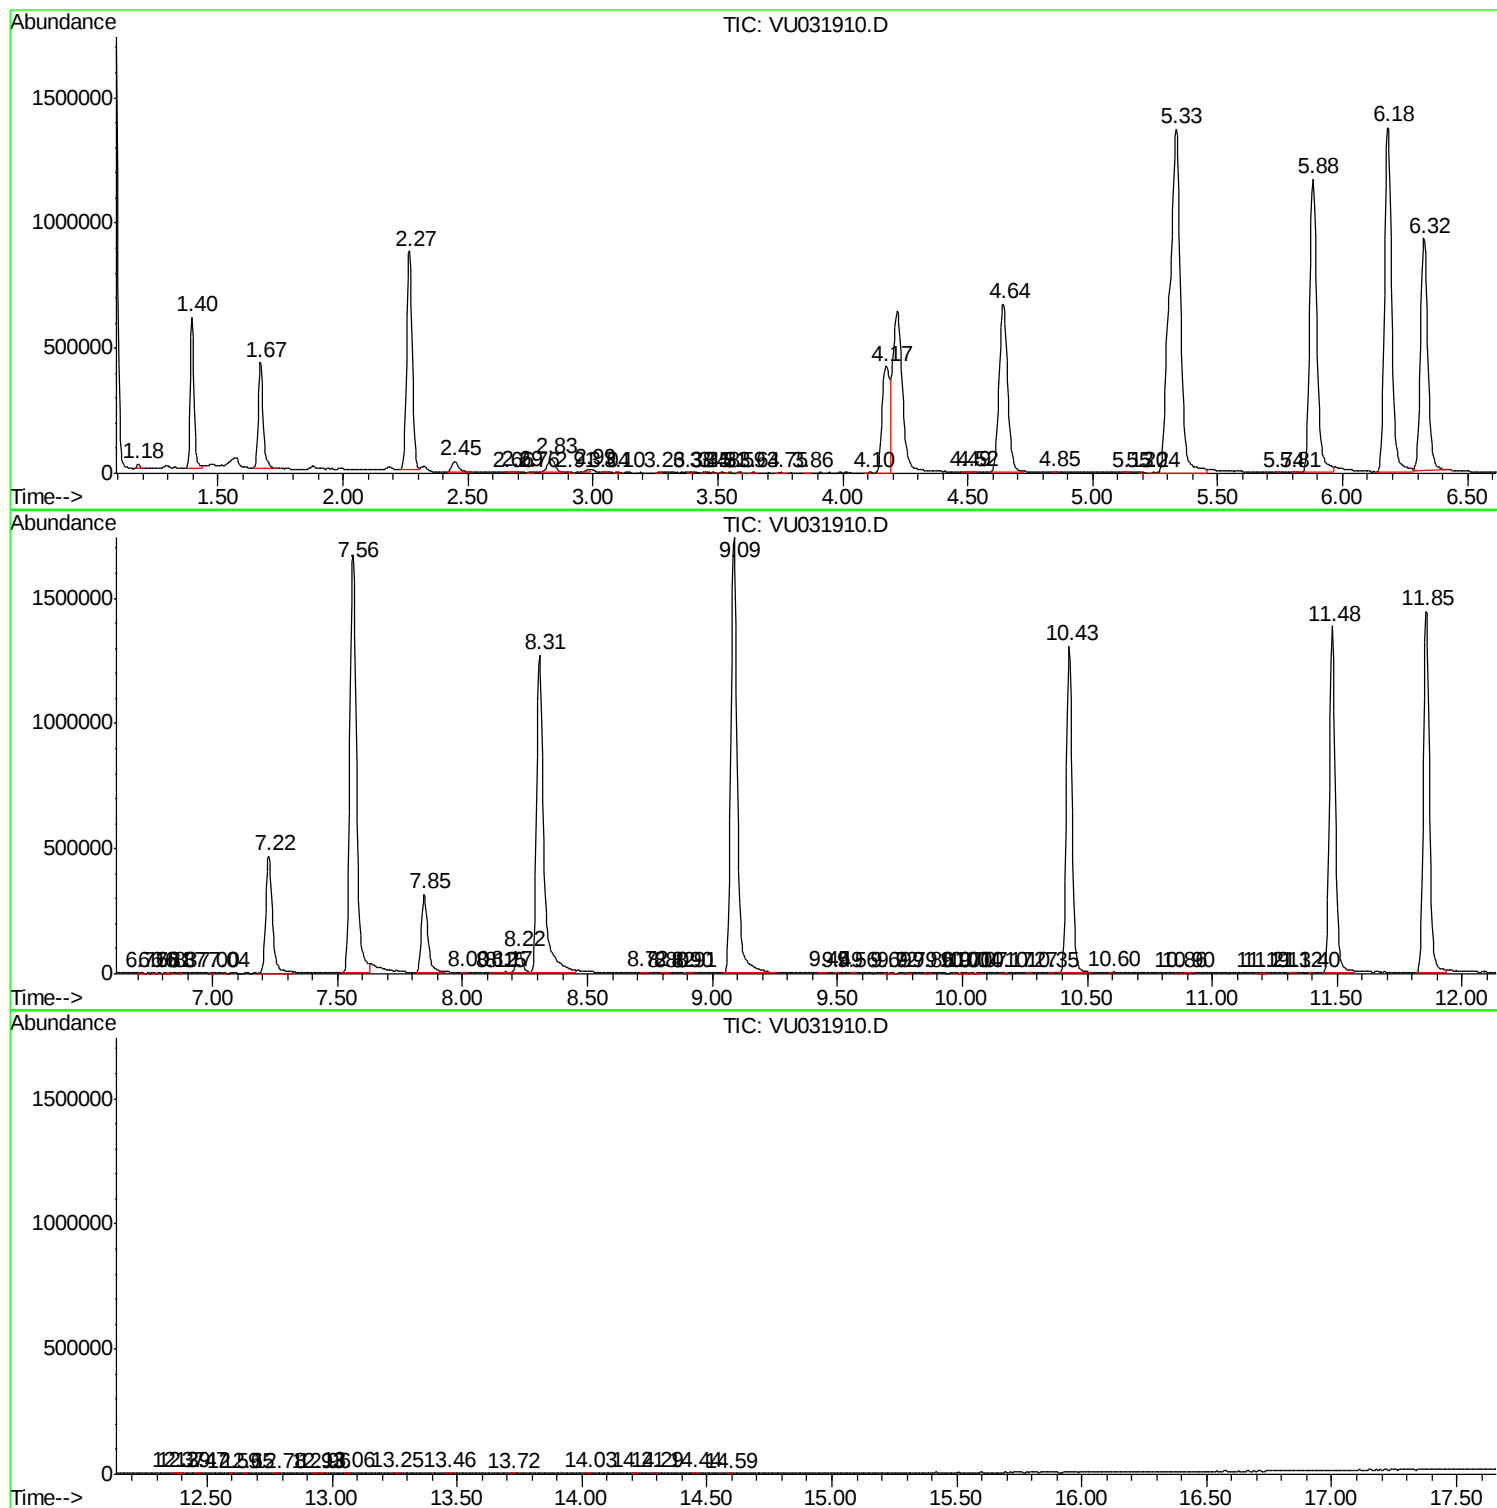

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031910.D
Acq On : 10 May 2019 23:53
Operator : JC/SP
Sample : K2705-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051019\
Data File : VU031910.D
Acq On : 10 May 2019 23:53
Operator : JC/SP
Sample : K2705-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B51

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc