


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051019\
 Data File : VU031876.D
 Acq On : 10 May 2019 10:07
 Operator : JC/SP
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Mon May 13 01:54:07 2019

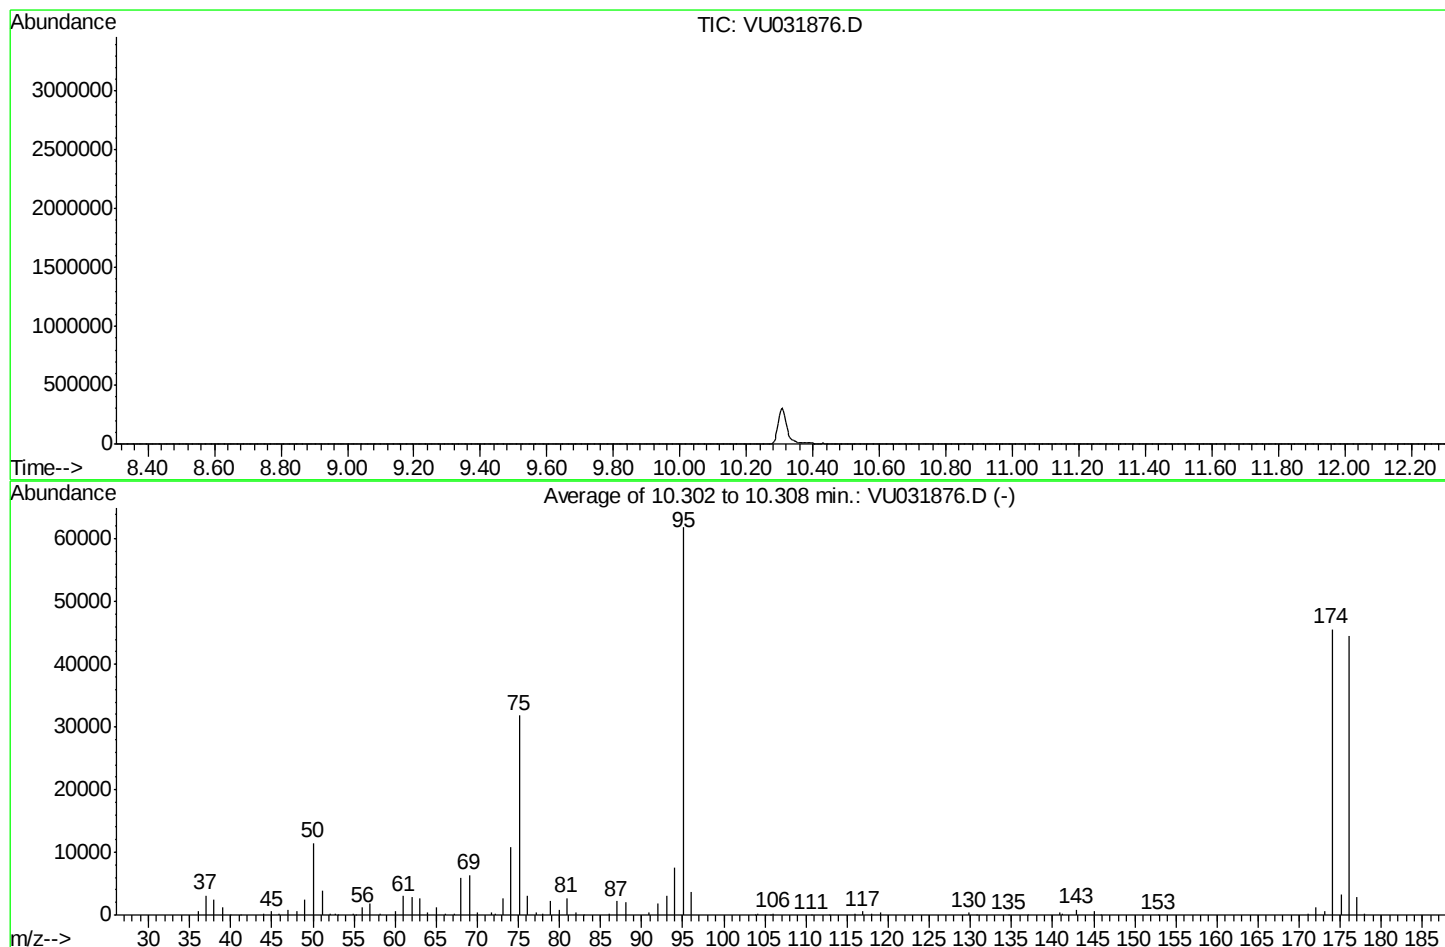

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	11463	PASS
75	95	30	80	51.4	31805	PASS
95	95	100	100	100.0	61853	PASS
96	95	5	9	5.9	3656	PASS
173	174	0.00	2	1.3	571	PASS
174	95	50	120	73.7	45584	PASS
175	174	5	9	7.2	3280	PASS
176	174	95	101	97.9	44610	PASS
177	176	5	9	6.6	2948	PASS

Scan 2854 (10.267 min): VU031876.D
BFB40

m/z	Abundance
39.90	1348.0
44.00	1293.0
45.00	127.0
68.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.10	618.0
37.00	2995.0
38.00	2389.0
39.00	1054.0
40.00	1635.0
41.20	130.0
44.00	1570.0
45.10	761.0
45.90	216.0
47.00	651.0
48.10	663.0
49.00	2110.0
50.00	11063.0
51.10	3564.0
52.10	195.0
52.80	229.0
54.90	185.0
56.00	1053.0
57.00	1653.0
58.10	122.0
60.10	697.0
61.00	2765.0
62.10	2753.0
63.00	2324.0
64.10	454.0
65.00	891.0
66.10	200.0
67.20	212.0
68.00	5831.0
69.10	6031.0
69.90	439.0
71.80	278.0
72.20	308.0
73.10	2539.0
74.10	10618.0
75.10	30688.0
76.00	2995.0
77.10	415.0
78.90	1927.0
79.90	760.0
80.90	2623.0
82.00	461.0
82.90	105.0
86.00	256.0
86.90	2250.0
88.00	1974.0
90.90	297.0
92.00	1752.0
93.00	2787.0
94.00	7292.0
95.10	58224.0
96.00	3499.0
103.80	190.0
106.00	288.0
110.70	108.0
116.00	226.0
117.00	526.0
117.90	186.0
119.00	402.0
129.80	327.0
130.80	143.0
136.90	108.0
140.90	508.0
142.90	772.0
145.00	526.0
145.90	130.0
152.90	201.0
171.00	176.0
172.00	1368.0
173.00	819.0
174.00	41752.0
175.00	3151.0
176.00	41168.0
177.00	2793.0
177.90	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.10	676.0
37.00	3153.0
38.00	2642.0
39.00	1315.0
40.00	1392.0
41.20	110.0
44.00	1542.0
45.00	755.0
45.90	247.0
47.00	786.0
48.10	686.0
49.00	2504.0
50.00	11780.0
51.10	3945.0
52.10	205.0
52.80	186.0
54.90	158.0
56.00	1198.0
57.00	1872.0
58.10	170.0
60.00	690.0
61.00	2985.0
62.10	2948.0
63.10	2583.0
63.90	488.0
65.00	1262.0
66.10	242.0
67.20	248.0
68.00	6043.0
69.10	6555.0
70.00	536.0
71.80	367.0
72.20	306.0
73.10	2838.0
74.10	11013.0
75.10	32752.0
76.00	3080.0
77.10	383.0
77.90	146.0
78.90	2189.0
79.90	777.0
80.90	2849.0
82.00	485.0
86.00	251.0
87.00	2217.0
88.00	2141.0
91.00	395.0
92.00	2001.0
93.00	3109.0
94.10	7733.0
95.10	63920.0
96.00	3753.0
104.10	177.0
105.00	121.0
106.00	287.0
112.90	125.0
116.00	196.0
116.90	572.0
117.90	201.0
119.00	414.0
129.80	372.0
130.80	103.0
134.70	126.0
140.80	406.0
142.90	852.0
145.00	550.0
152.90	126.0
171.00	353.0
172.00	1363.0
173.10	895.0
174.00	46688.0
175.00	3312.0
176.00	46344.0
177.00	3034.0
177.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.10	555.0
37.00	3162.0
38.00	2554.0
39.10	1347.0
40.00	1324.0
44.00	1634.0
45.00	619.0
45.90	223.0
47.00	812.0
48.10	624.0
49.00	2733.0
50.00	11546.0
51.10	3930.0
52.10	220.0
53.00	136.0
54.80	162.0
55.20	207.0
56.00	1144.0
57.00	1945.0
58.10	154.0
60.00	692.0
61.00	3248.0
62.00	2985.0
63.10	2845.0
63.90	528.0
65.10	1360.0
66.10	217.0
67.20	288.0
68.00	5847.0
69.10	6738.0
70.00	564.0
71.80	452.0
73.10	2741.0
74.00	10614.0
75.10	31976.0
76.10	2891.0
77.10	326.0
77.90	239.0
79.00	2437.0
79.90	714.0
80.90	2506.0
81.90	467.0
87.00	2040.0
88.10	2246.0
91.00	419.0
92.00	1877.0
93.00	3023.0
94.10	7472.0
95.10	63416.0
96.10	3717.0
104.10	260.0
105.00	129.0
105.70	283.0
106.00	285.0
112.90	113.0
116.00	131.0
116.90	502.0
118.00	204.0
119.00	432.0
129.90	323.0
134.70	115.0
140.80	353.0
141.10	392.0
143.00	957.0
145.00	487.0
171.00	406.0
172.00	1122.0
174.00	48312.0
175.10	3378.0
176.00	46320.0
177.00	3019.0
177.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40