

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043627.D
 Acq On : 10 May 2021 10:36
 Operator : SY/MD
 Sample : VU0510WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK147

Quant Time: May 11 03:58:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 11 03:58:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	103630	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	100647	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	46594	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	30915	3.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.20%
7) Chloroethane-d5	1.916	69	24912	4.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.60%
11) 1,1-Dichloroethene-d2	2.572	65	15723	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.80%
20) 2-Butanone-d5	4.646	46	132392	51.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.36%
24) Chloroform-d	5.073	84	69092	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
26) 1,2-Dichloroethane-d4	5.710	65	44640	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.736	84	127464	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.700	67	46359	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	7.906	98	108665	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloroprop...	8.186	79	18297	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.642	63	90005	55.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.44%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	36946	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
66) 1,2-Dichlorobenzene-d4	12.201	152	40951	4.93	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.60%
Target Compounds						
16) Methylene chloride	3.054	84	5584	0.60	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043627.D
Acq On : 10 May 2021 10:36
Operator : SY/MD
Sample : VU0510WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK147

Quant Time: May 11 03:58:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 11 03:58:06 2021
Response via : Initial Calibration

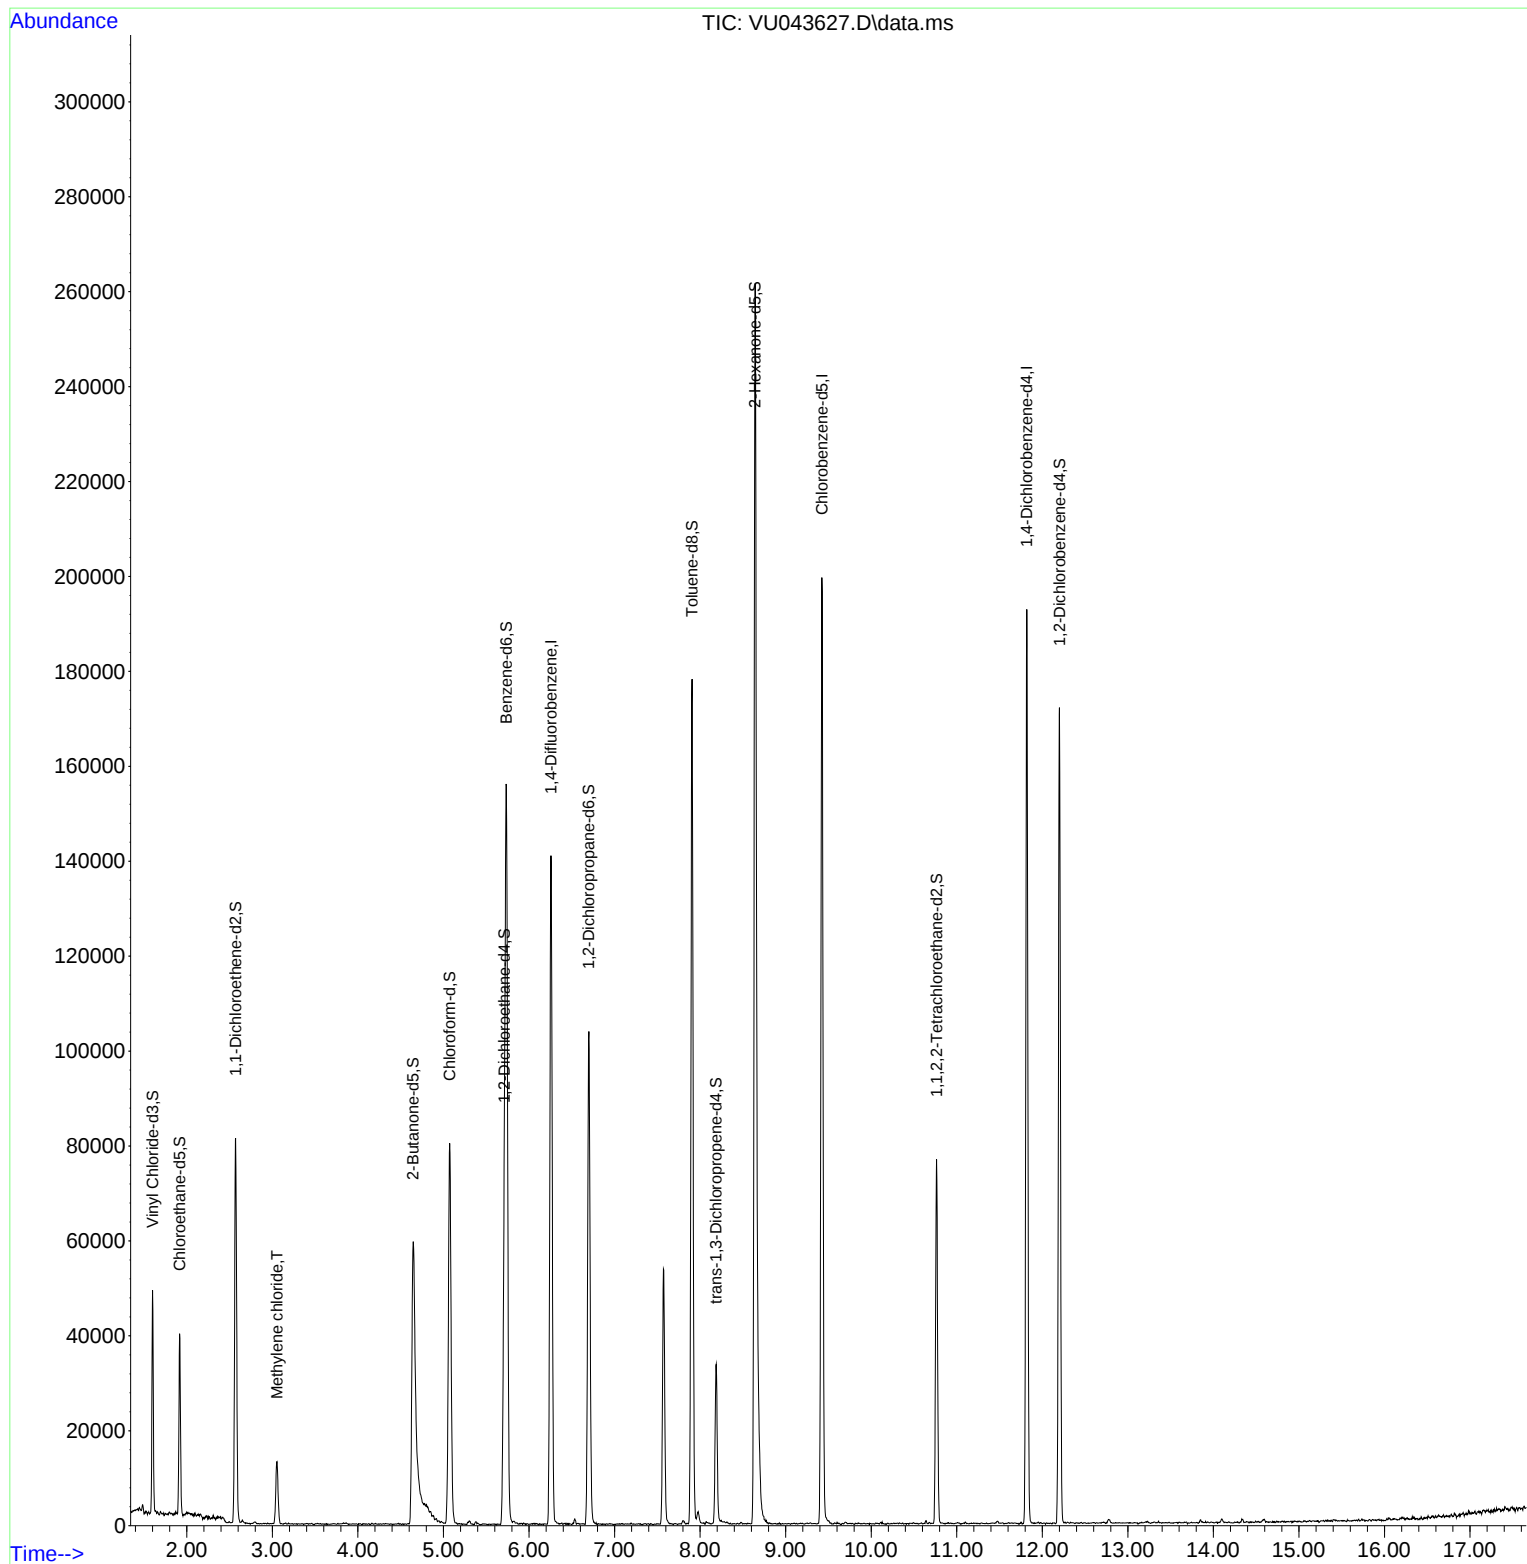

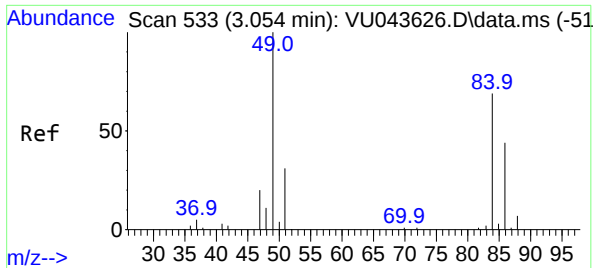

#16
Methylene chloride
Concen: 0.60 ug/L
RT: 3.054 min Scan# 533
Delta R.T. 0.000 min
Lab File: VU043627.D
Acq: 10 May 2021 10:36

Instrument :
MSVOA_U
ClientSampleId :
VBLK147

Tgt Ion: 84 Resp: 5584

Ion	Ratio	Lower	Upper
84	100		
86	63.4	45.6	84.6
49	141.7	107.0	198.8

