

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043641.D
 Acq On : 10 May 2021 16:18
 Operator : SY/MD
 Sample : M2272-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Quant Time: May 11 03:59:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 11 03:58:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	97352	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	94750	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	42660	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	27937	3.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.40%
7) Chloroethane-d5	1.919	69	23808	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.00%
11) 1,1-Dichloroethene-d2	2.571	65	14739	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.80%
20) 2-Butanone-d5	4.642	46	111162	45.74	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.48%
24) Chloroform-d	5.073	84	66862	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.713	65	42871	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.735	84	121575	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.700	67	44787	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.906	98	100529	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
43) trans-1,3-Dichloroprop...	8.189	79	16182	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.645	63	87808	57.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.48%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	37125	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
66) 1,2-Dichlorobenzene-d4	12.201	152	37406	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	2414	0.28	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043641.D
Acq On : 10 May 2021 16:18
Operator : SY/MD
Sample : M2272-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Time: May 11 03:59:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 11 03:58:06 2021
Response via : Initial Calibration

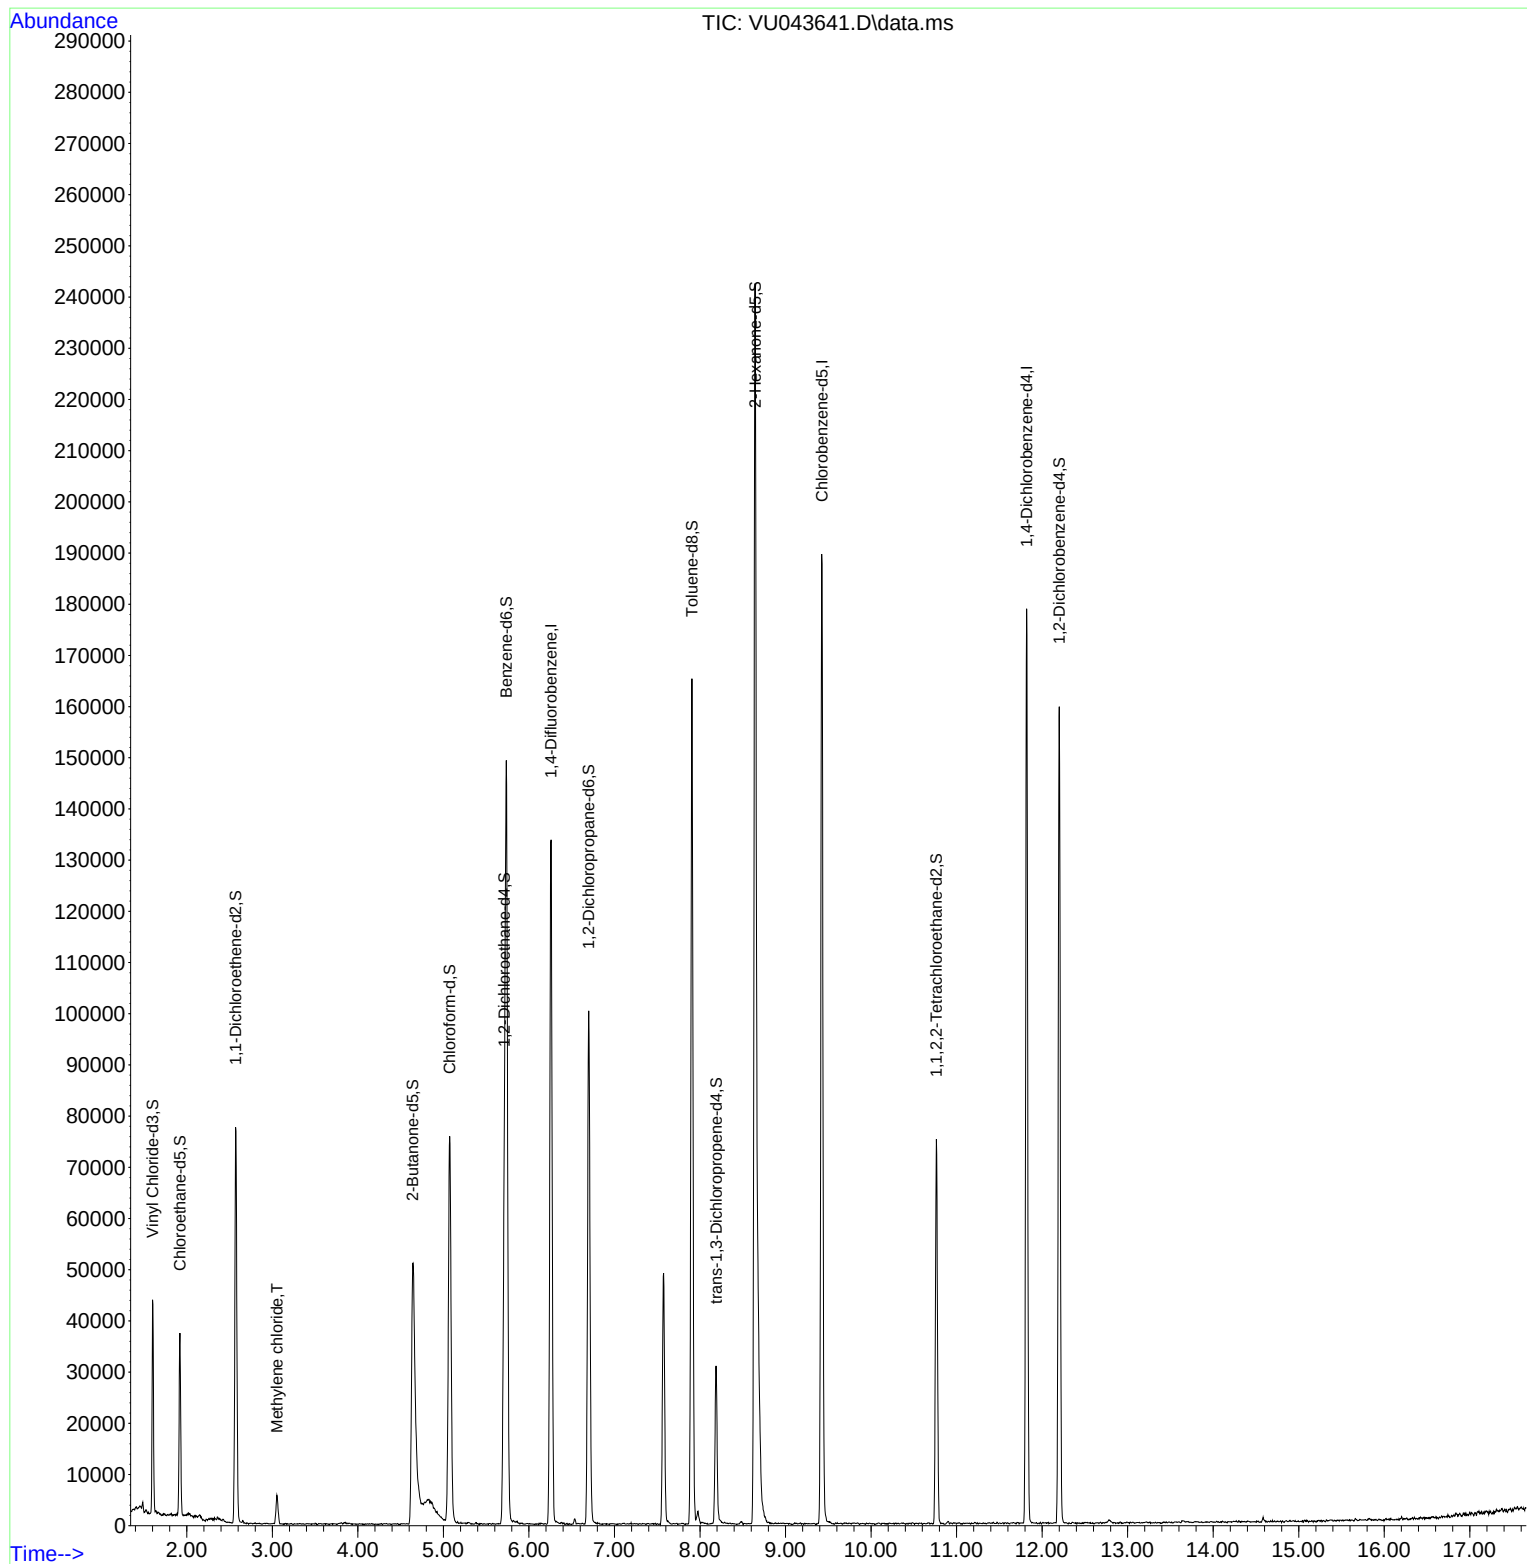

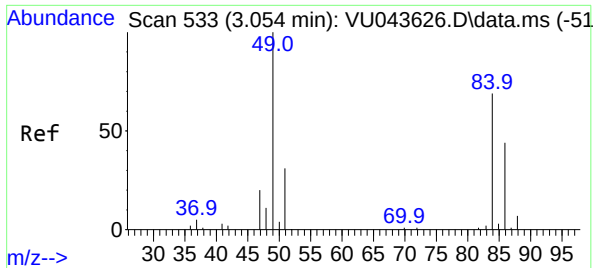

#16
Methylene chloride
Concen: 0.28 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU043641.D
Acq: 10 May 2021 16:18

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Tgt Ion:	84	Resp:	2414
Ion	Ratio	Lower	Upper
84	100		
86	56.9	45.6	84.6
49	129.4	107.0	198.8

