

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043637.D
 Acq On : 10 May 2021 14:42
 Operator : SY/MD
 Sample : M2320-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3A04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	52	rVB	7244	7754	1.45%	0.225%
2	1.604	73	82	98	rBV	41690	48850	9.12%	1.418%
3	1.919	171	180	192	rBV	35569	45346	8.46%	1.317%
4	2.572	371	383	399	rBV	74790	121351	22.64%	3.524%
5	2.671	399	414	419	rBV3	3545	8464	1.58%	0.246%
6	3.195	564	577	591	rBV	4510	9258	1.73%	0.269%
7	4.658	1014	1032	1082	rBV2	64186	256052	47.78%	7.435%
8	5.073	1143	1161	1194	rBV	75896	172255	32.14%	5.002%
9	5.735	1345	1367	1388	rBV2	144531	380035	70.91%	11.035%
10	6.260	1515	1530	1547	rBV	134526	250241	46.69%	7.266%
11	6.700	1654	1667	1685	rVB2	97802	188960	35.26%	5.487%
12	7.575	1926	1939	1957	rBV	49329	86934	16.22%	2.524%
13	7.906	2026	2042	2056	rBV	164527	275931	51.49%	8.012%
14	7.977	2056	2064	2073	rVB2	4815	7955	1.48%	0.231%
15	8.186	2118	2129	2145	rBV2	31738	52492	9.79%	1.524%
16	8.645	2259	2272	2309	rBV	268792	535912	100.00%	15.561%
17	9.423	2501	2514	2530	rBV	194766	315352	58.84%	9.157%
18	10.764	2919	2931	2947	rBV	74214	118311	22.08%	3.435%
19	11.819	3248	3259	3273	rBV	180898	285811	53.33%	8.299%
20	12.066	3329	3336	3346	rBV4	4391	6896	1.29%	0.200%
21	12.201	3365	3378	3395	rVB	159634	255978	47.76%	7.433%
22	12.896	3586	3594	3603	rBV5	9610	13870	2.59%	0.403%




Sum of corrected areas: 3444008

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043637.D
Acq On : 10 May 2021 14:42
Operator : SY/MD
Sample : M2320-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

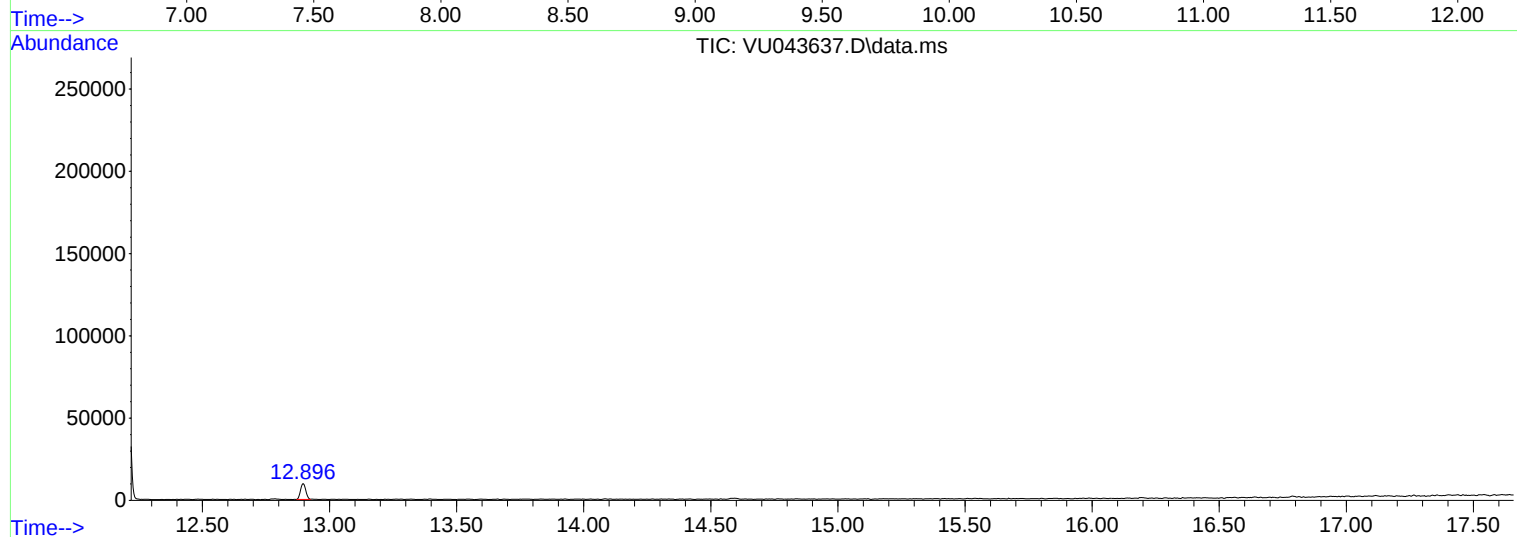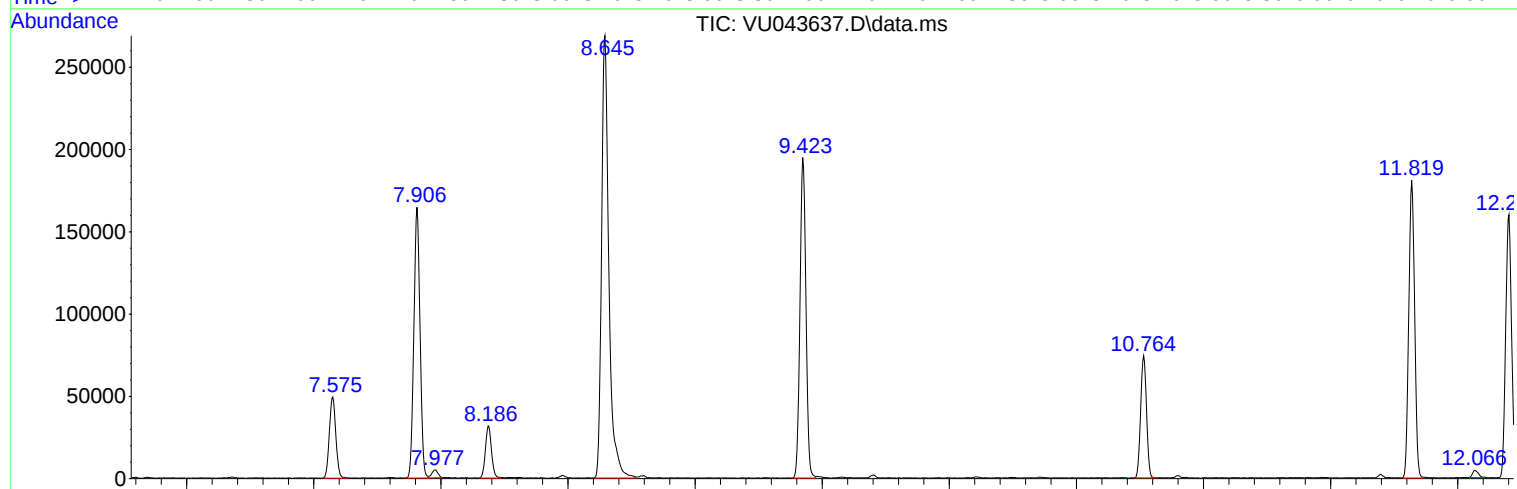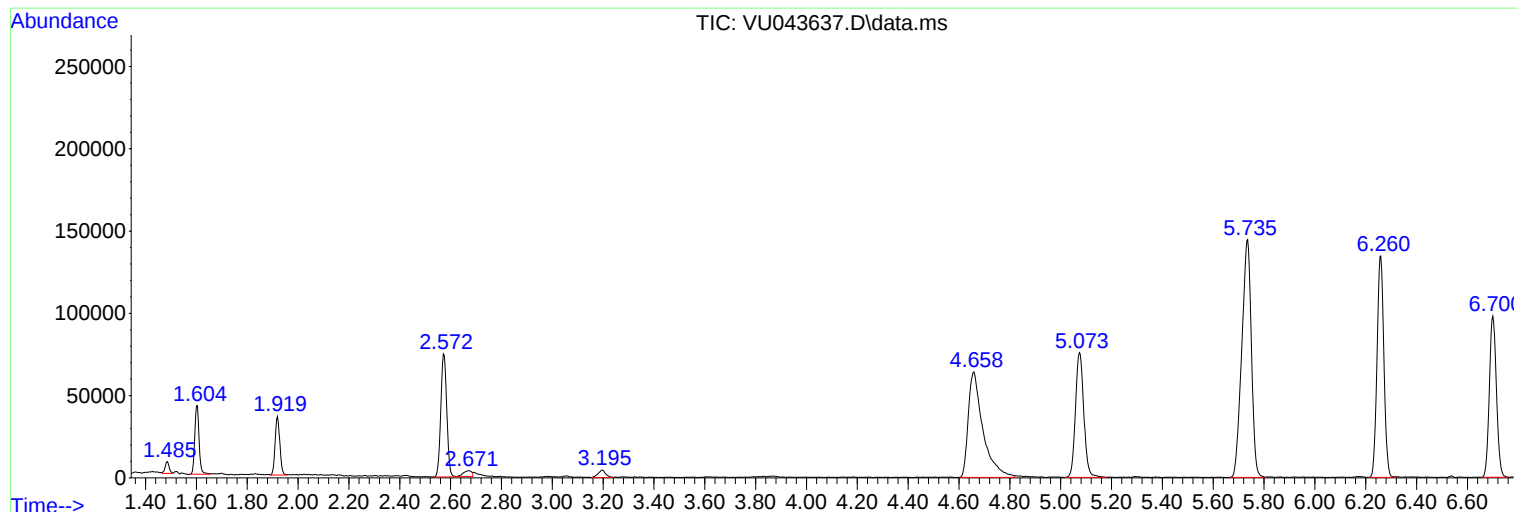

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043637.D
Acq On : 10 May 2021 14:42
Operator : SY/MD
Sample : M2320-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043637.D
Acq On : 10 May 2021 14:42
Operator : SY/MD
Sample : M2320-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
