

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043638.D
 Acq On : 10 May 2021 15:06
 Operator : SY/MD
 Sample : M2320-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3A10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rVB	6872	6590	1.25%	0.196%
2	1.601	73	81	93	rBV	40560	45246	8.57%	1.349%
3	1.919	172	180	192	rVB	35895	44828	8.49%	1.336%
4	2.572	371	383	397	rBV	74081	119243	22.57%	3.555%
5	2.665	400	412	415	rBV4	3685	6601	1.25%	0.197%
6	4.655	1011	1031	1070	rBV2	57625	224305	42.46%	6.686%
7	5.073	1145	1161	1184	rBV	75579	168430	31.88%	5.021%
8	5.735	1344	1367	1390	rBV2	141988	372061	70.43%	11.091%
9	6.256	1515	1529	1545	rBV	132579	246644	46.69%	7.352%
10	6.700	1651	1667	1683	rBV	96391	186460	35.30%	5.558%
11	7.575	1927	1939	1957	rVB	49920	85190	16.13%	2.539%
12	7.906	2029	2042	2056	rBV	160322	273124	51.70%	8.142%
13	7.976	2057	2064	2076	rVB3	4581	7587	1.44%	0.226%
14	8.189	2119	2130	2148	rBV	30862	52158	9.87%	1.555%
15	8.645	2259	2272	2311	rBV	267978	528249	100.00%	15.747%
16	9.423	2501	2514	2534	rBV	189739	311578	58.98%	9.288%
17	10.764	2920	2931	2945	rBV	74475	118084	22.35%	3.520%
18	11.819	3247	3259	3278	rVB	180830	283155	53.60%	8.441%
19	12.066	3328	3336	3347	rBV5	5424	8838	1.67%	0.263%
20	12.201	3366	3378	3394	rVB	158824	251603	47.63%	7.500%
21	12.896	3583	3594	3603	rBV3	10507	14721	2.79%	0.439%




Sum of corrected areas: 3354695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043638.D
Acq On : 10 May 2021 15:06
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

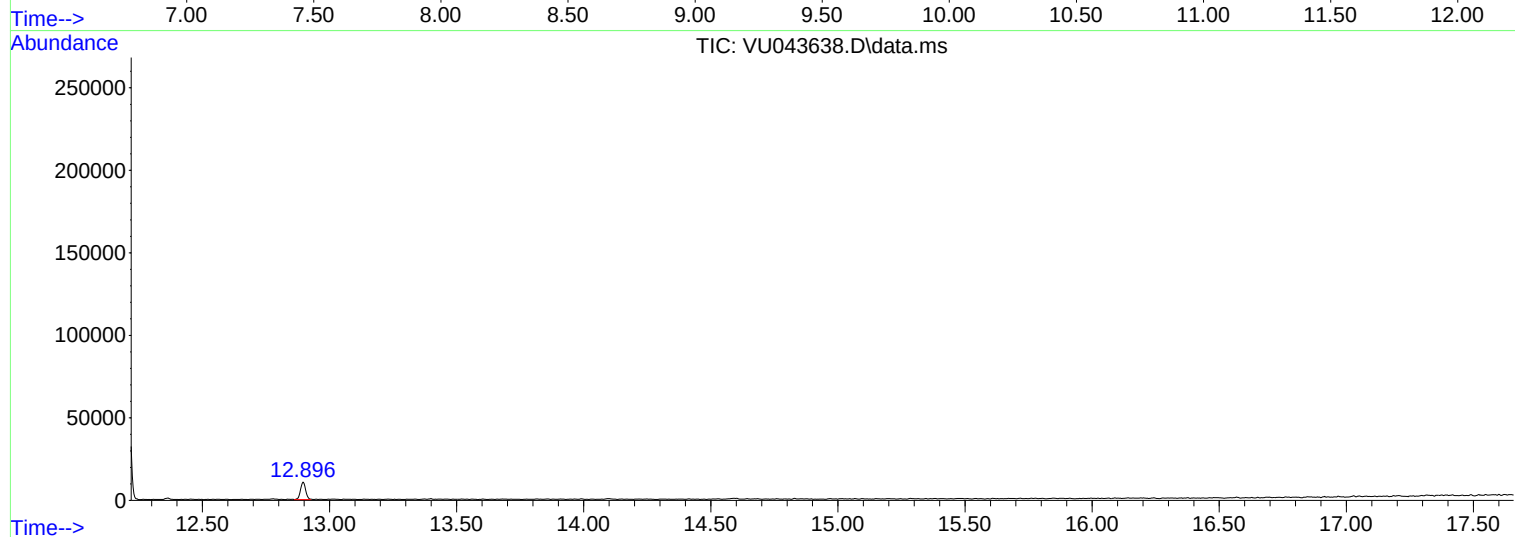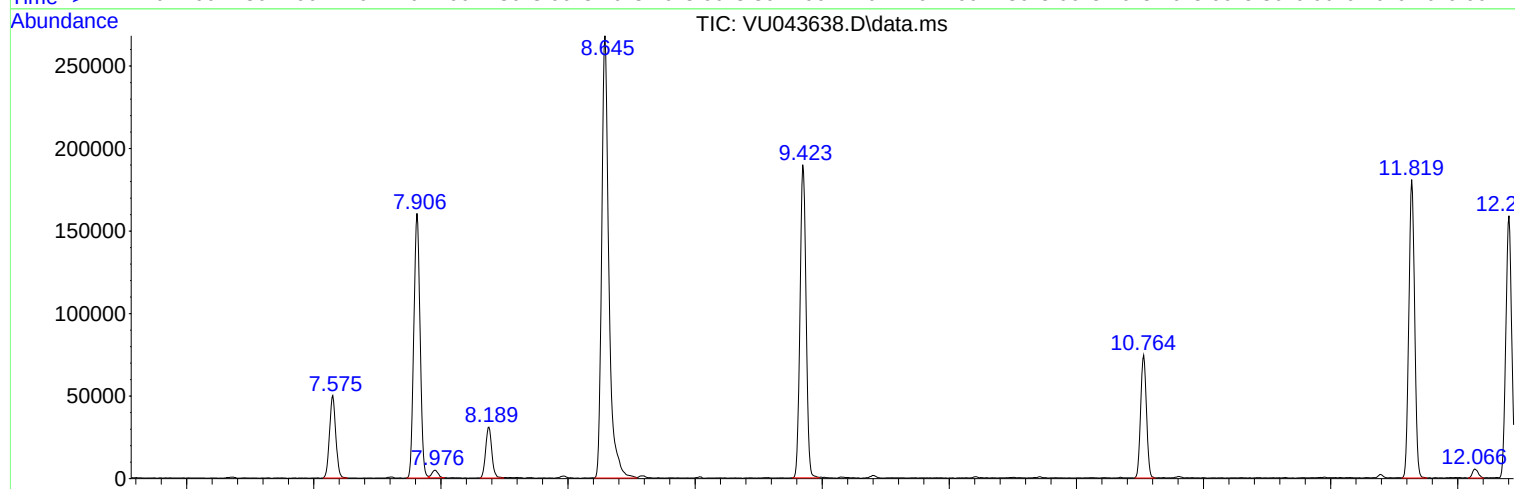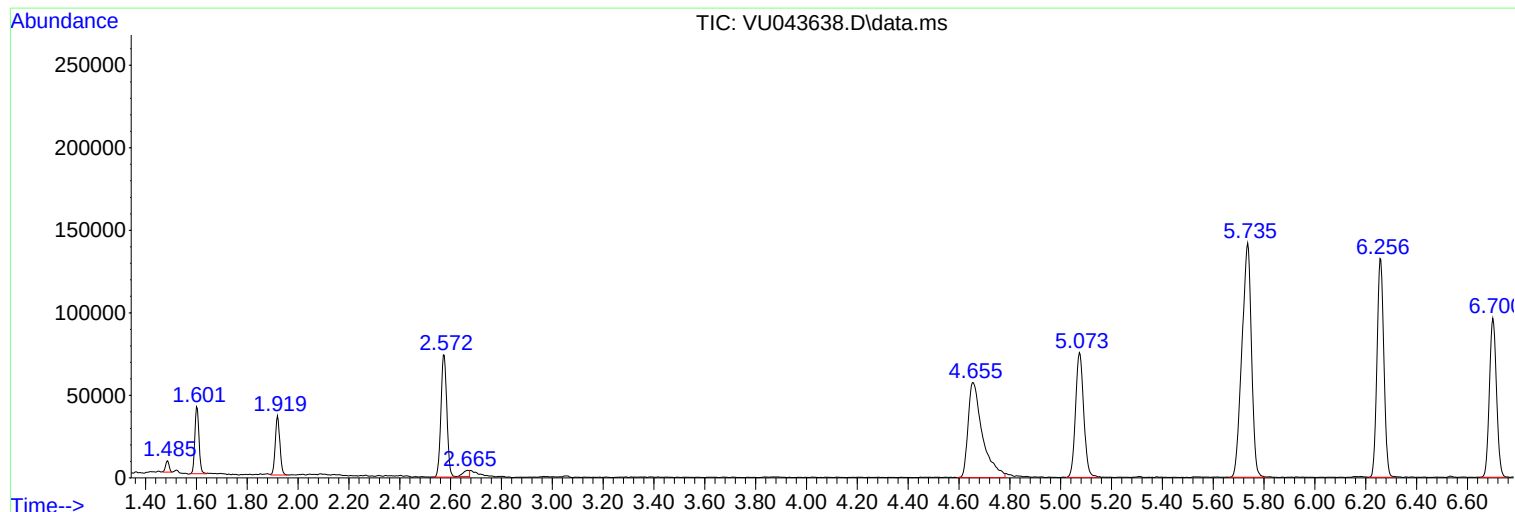

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043638.D
Acq On : 10 May 2021 15:06
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043638.D
Acq On : 10 May 2021 15:06
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc