

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043644.D
 Acq On : 10 May 2021 17:31
 Operator : SY/MD
 Sample : M2300-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6B7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	90	rBV	39001	45400	8.39%	1.357%
2	1.919	172	180	194	rVB	34864	44793	8.28%	1.339%
3	2.575	371	384	403	rBV	70643	116829	21.60%	3.492%
4	3.054	521	533	543	rBV3	4089	6646	1.23%	0.199%
5	4.645	1011	1028	1067	rBV	77811	227981	42.14%	6.815%
6	5.073	1144	1161	1183	rVB	76533	169029	31.25%	5.053%
7	5.735	1346	1367	1387	rBV2	140217	371479	68.67%	11.105%
8	6.256	1515	1529	1548	rBV	134079	249070	46.04%	7.446%
9	6.700	1653	1667	1686	rBV2	98880	188348	34.82%	5.630%
10	7.575	1926	1939	1956	rVB	47841	83430	15.42%	2.494%
11	7.906	2030	2042	2056	rBV	157226	268233	49.59%	8.018%
12	7.976	2057	2064	2079	rVB2	4336	7356	1.36%	0.220%
13	8.185	2119	2129	2143	rBV	30992	51572	9.53%	1.542%
14	8.642	2259	2271	2307	rBV	285089	540953	100.00%	16.171%
15	9.423	2502	2514	2535	rBV	190953	314332	58.11%	9.396%
16	9.603	2554	2570	2583	rVB2	8817	14214	2.63%	0.425%
17	9.700	2591	2600	2608	rVB3	4086	5832	1.08%	0.174%
18	10.764	2920	2931	2945	rBV	76700	119975	22.18%	3.586%
19	11.819	3247	3259	3277	rBV	174351	274316	50.71%	8.200%
20	12.201	3366	3378	3392	rBV	155057	245452	45.37%	7.337%




Sum of corrected areas: 3345240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043644.D
Acq On : 10 May 2021 17:31
Operator : SY/MD
Sample : M2300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

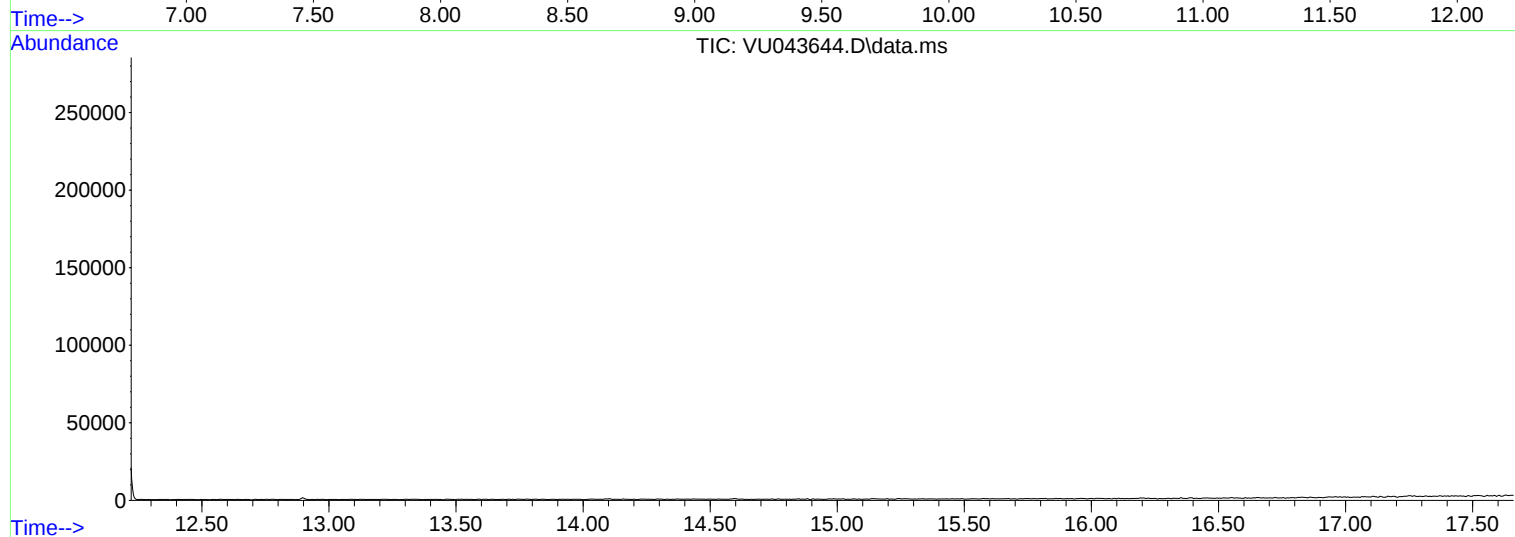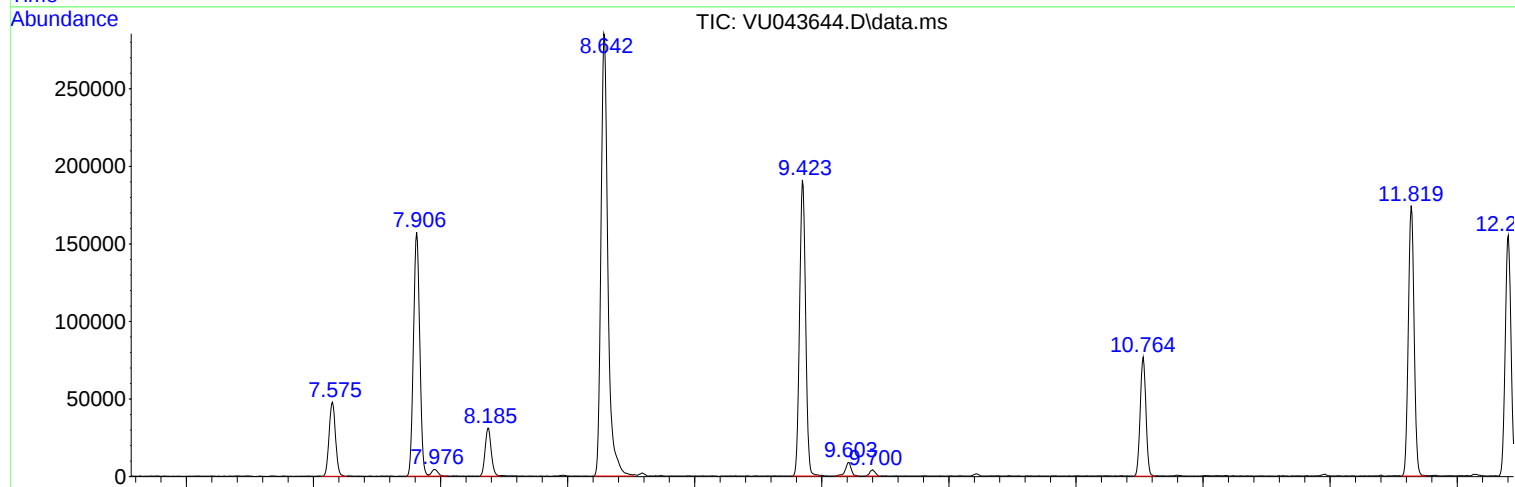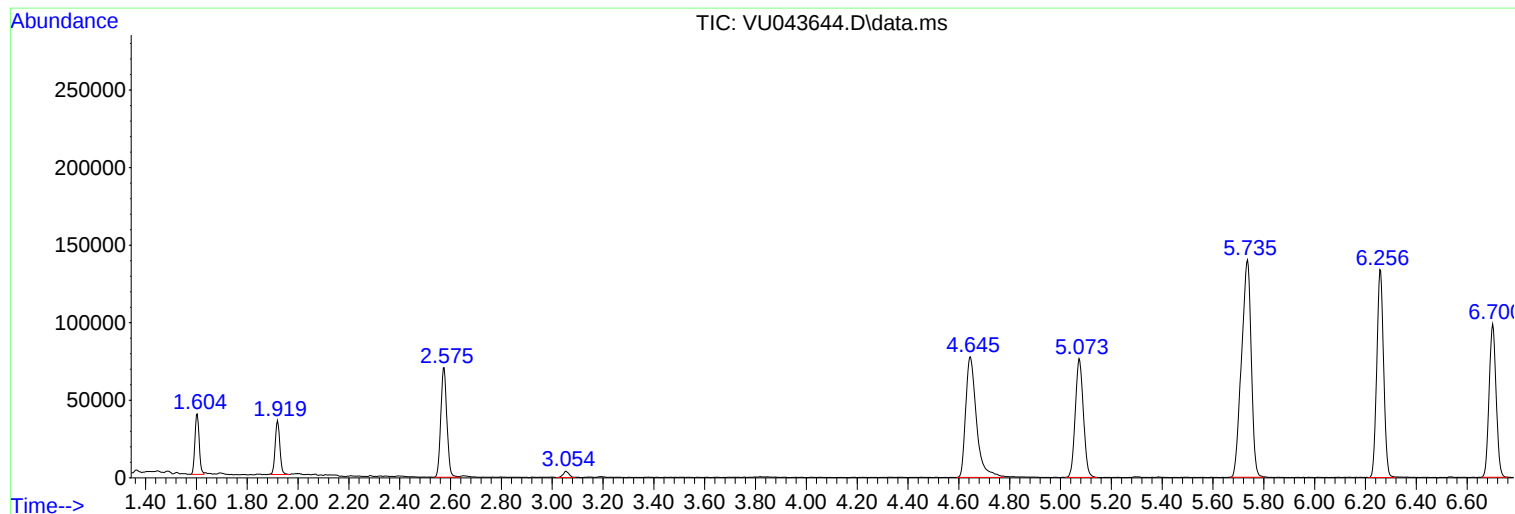

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043644.D
Acq On : 10 May 2021 17:31
Operator : SY/MD
Sample : M2300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
Data File : VU043644.D
Acq On : 10 May 2021 17:31
Operator : SY/MD
Sample : M2300-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
