
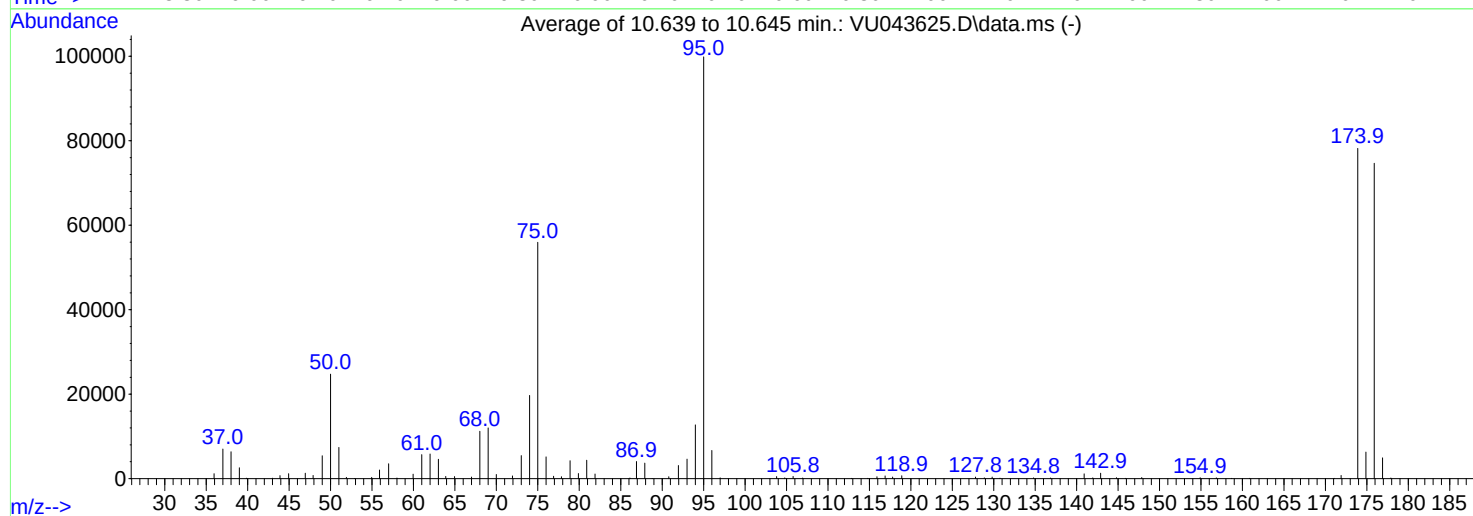


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051021\
 Data File : VU043625.D
 Acq On : 10 May 2021 09:06
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB141

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 11 03:58:06 2021

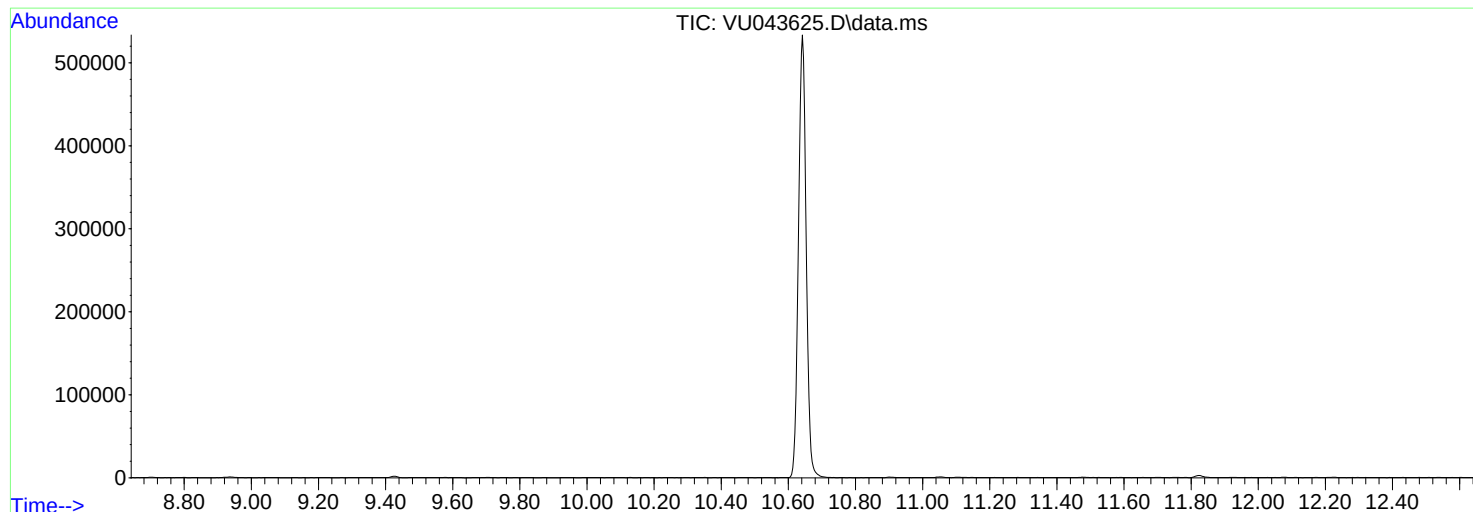

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	24741	PASS
75	95	30	80	56.0	55944	PASS
95	95	100	100	100.0	99867	PASS
96	95	5	9	6.7	6680	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.3	78208	PASS
175	174	5	9	8.0	6284	PASS
176	174	95	101	95.5	74672	PASS
177	176	5	9	6.6	4942	PASS

m/z	Abundance
35.90	1135.0
37.00	6952.0
38.00	6138.0
39.00	2541.0
39.90	227.0
43.00	113.0
43.90	977.0
45.00	1050.0
46.90	1250.0
47.90	790.0
49.00	5165.0
50.00	23776.0
51.00	7099.0
51.90	283.0
55.00	305.0
55.90	1937.0
57.00	3374.0
58.00	109.0
60.00	1079.0
61.00	5472.0
62.00	5611.0
63.00	4351.0
63.90	494.0
64.90	481.0
67.00	355.0
68.00	10832.0
69.00	11408.0
70.00	944.0
71.90	591.0
73.00	5239.0
74.00	19040.0
75.00	53848.0
76.00	4959.0
76.90	605.0
77.90	404.0
78.90	3967.0
79.90	1155.0
80.90	4133.0
81.90	1029.0
86.90	3960.0
87.90	3630.0
90.80	467.0
91.90	3074.0
93.00	4425.0
94.00	12518.0
95.00	97472.0
96.00	6661.0
97.00	141.0
103.80	455.0
104.80	206.0
105.80	511.0
107.00	130.0
115.90	466.0
116.90	679.0
117.80	408.0
118.90	696.0
127.80	376.0
128.90	161.0
129.80	312.0
130.70	137.0
134.80	178.0
136.80	179.0
140.90	1141.0
142.00	147.0
142.90	1267.0
144.80	208.0
145.90	146.0
147.90	240.0
154.90	212.0
156.80	211.0
160.80	140.0
171.90	735.0
173.90	78928.0
174.90	6222.0
175.90	74272.0
176.90	5041.0
177.90	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
39.90	118.0
43.90	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
36.00	1193.0
37.00	6849.0
38.00	6376.0
39.00	2529.0
39.80	234.0
43.00	112.0
43.90	926.0
44.90	1245.0
47.00	1301.0
47.90	705.0
49.00	5506.0
50.00	24792.0
51.00	7411.0
51.90	349.0
52.90	102.0
54.90	283.0
55.90	2058.0
57.00	3514.0
58.00	155.0
59.90	1046.0
61.00	5736.0
62.00	5875.0
63.00	4645.0
63.90	564.0
65.00	547.0
67.00	415.0
68.00	11211.0
69.00	12289.0
70.00	973.0
72.00	692.0
73.00	5500.0
74.00	19808.0
75.00	56336.0
76.00	5139.0
76.90	558.0
77.80	517.0
78.90	4394.0
79.90	1283.0
80.90	4461.0
81.90	1110.0
86.10	210.0
86.90	4007.0
87.90	3657.0
88.80	135.0
90.80	440.0
92.00	3075.0
93.00	4633.0
94.00	12621.0
95.00	99128.0
96.00	6522.0
97.00	222.0
103.80	552.0
104.80	161.0
105.80	513.0
106.90	140.0
112.80	142.0
114.80	129.0
115.90	426.0
116.90	641.0
117.80	324.0
118.90	694.0
127.80	374.0
128.80	214.0
129.80	411.0
130.80	105.0
134.80	178.0
136.90	129.0
140.90	1114.0
141.90	197.0
142.90	1272.0
144.80	261.0
147.80	255.0
154.90	214.0
156.90	209.0
158.70	114.0
171.00	141.0
171.90	762.0
173.90	75120.0
174.90	6153.0
175.90	72664.0
176.90	4699.0
177.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
36.00	1230.0
37.00	7286.0
38.00	6593.0
39.00	2612.0
39.80	242.0
43.00	126.0
43.90	962.0
44.90	1200.0
46.90	1367.0
47.90	796.0
49.00	5645.0
50.00	25656.0
51.00	7711.0
51.90	319.0
55.00	289.0
55.90	2176.0
57.00	3641.0
58.00	144.0
59.90	1110.0
61.00	5897.0
62.00	6041.0
63.00	4766.0
63.90	563.0
65.00	518.0
67.00	409.0
68.00	11636.0
69.00	12328.0
70.00	1005.0
72.00	649.0
73.00	5659.0
74.00	20232.0
75.00	57648.0
76.00	5336.0
76.90	603.0
77.90	483.0
78.90	4351.0
79.90	1246.0
80.90	4541.0
81.90	1120.0
86.10	202.0
86.90	4228.0
87.90	3748.0
90.80	477.0
92.00	3191.0
93.00	4755.0
94.00	13100.0
95.00	103000.0
96.00	6857.0
97.00	199.0
103.80	534.0
104.80	199.0
105.80	541.0
106.90	147.0
112.90	126.0
114.80	127.0
115.90	469.0
116.90	672.0
117.80	388.0
118.90	693.0
127.80	387.0
128.80	206.0
129.80	391.0
130.70	121.0
134.80	182.0
136.80	150.0
140.90	1168.0
141.90	178.0
142.90	1324.0
144.80	242.0
145.90	114.0
147.80	251.0
154.90	235.0
156.90	202.0
158.70	109.0
160.90	117.0
171.10	128.0
171.90	777.0
173.90	80576.0
174.90	6478.0
175.90	77080.0
176.90	5086.0
177.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141