

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048485.D
 Acq On : 10 May 2022 12:54
 Operator : SY/MD
 Sample : N2736-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW1

Quant Time: May 11 05:21:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 05:17:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	277028	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	277054	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	139294	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	89629	37.567	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.140%
7) Chloroethane-d5	1.912	69	71244	45.755	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.520%
11) 1,1-Dichloroethene-d2	2.568	63	144023	33.919	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.840%
21) 2-Butanone-d5	4.620	46	168379	82.870	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.870%
24) Chloroform-d	5.063	84	199498	48.141	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.280%
26) 1,2-Dichloroethane-d4	5.703	65	143267	53.185	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.360%
32) Benzene-d6	5.729	84	379442	45.069	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.140%
36) 1,2-Dichloropropane-d6	6.690	67	118563	43.185	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.380%
41) Toluene-d8	7.899	98	337577	45.337	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.680%
43) trans-1,3-Dichloroprop...	8.179	79	43898	34.739	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.480%
47) 2-Hexanone-d5	8.632	63	124127	93.411	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.410%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	176020	42.090	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.180%
66) 1,2-Dichlorobenzene-d4	12.192	152	133535	48.413	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.820%
Target Compounds						
33) Benzene	5.777	78	12175	1.276	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048485.D
Acq On : 10 May 2022 12:54
Operator : SY/MD
Sample : N2736-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW1

Quant Time: May 11 05:21:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 05:17:27 2022
Response via : Initial Calibration

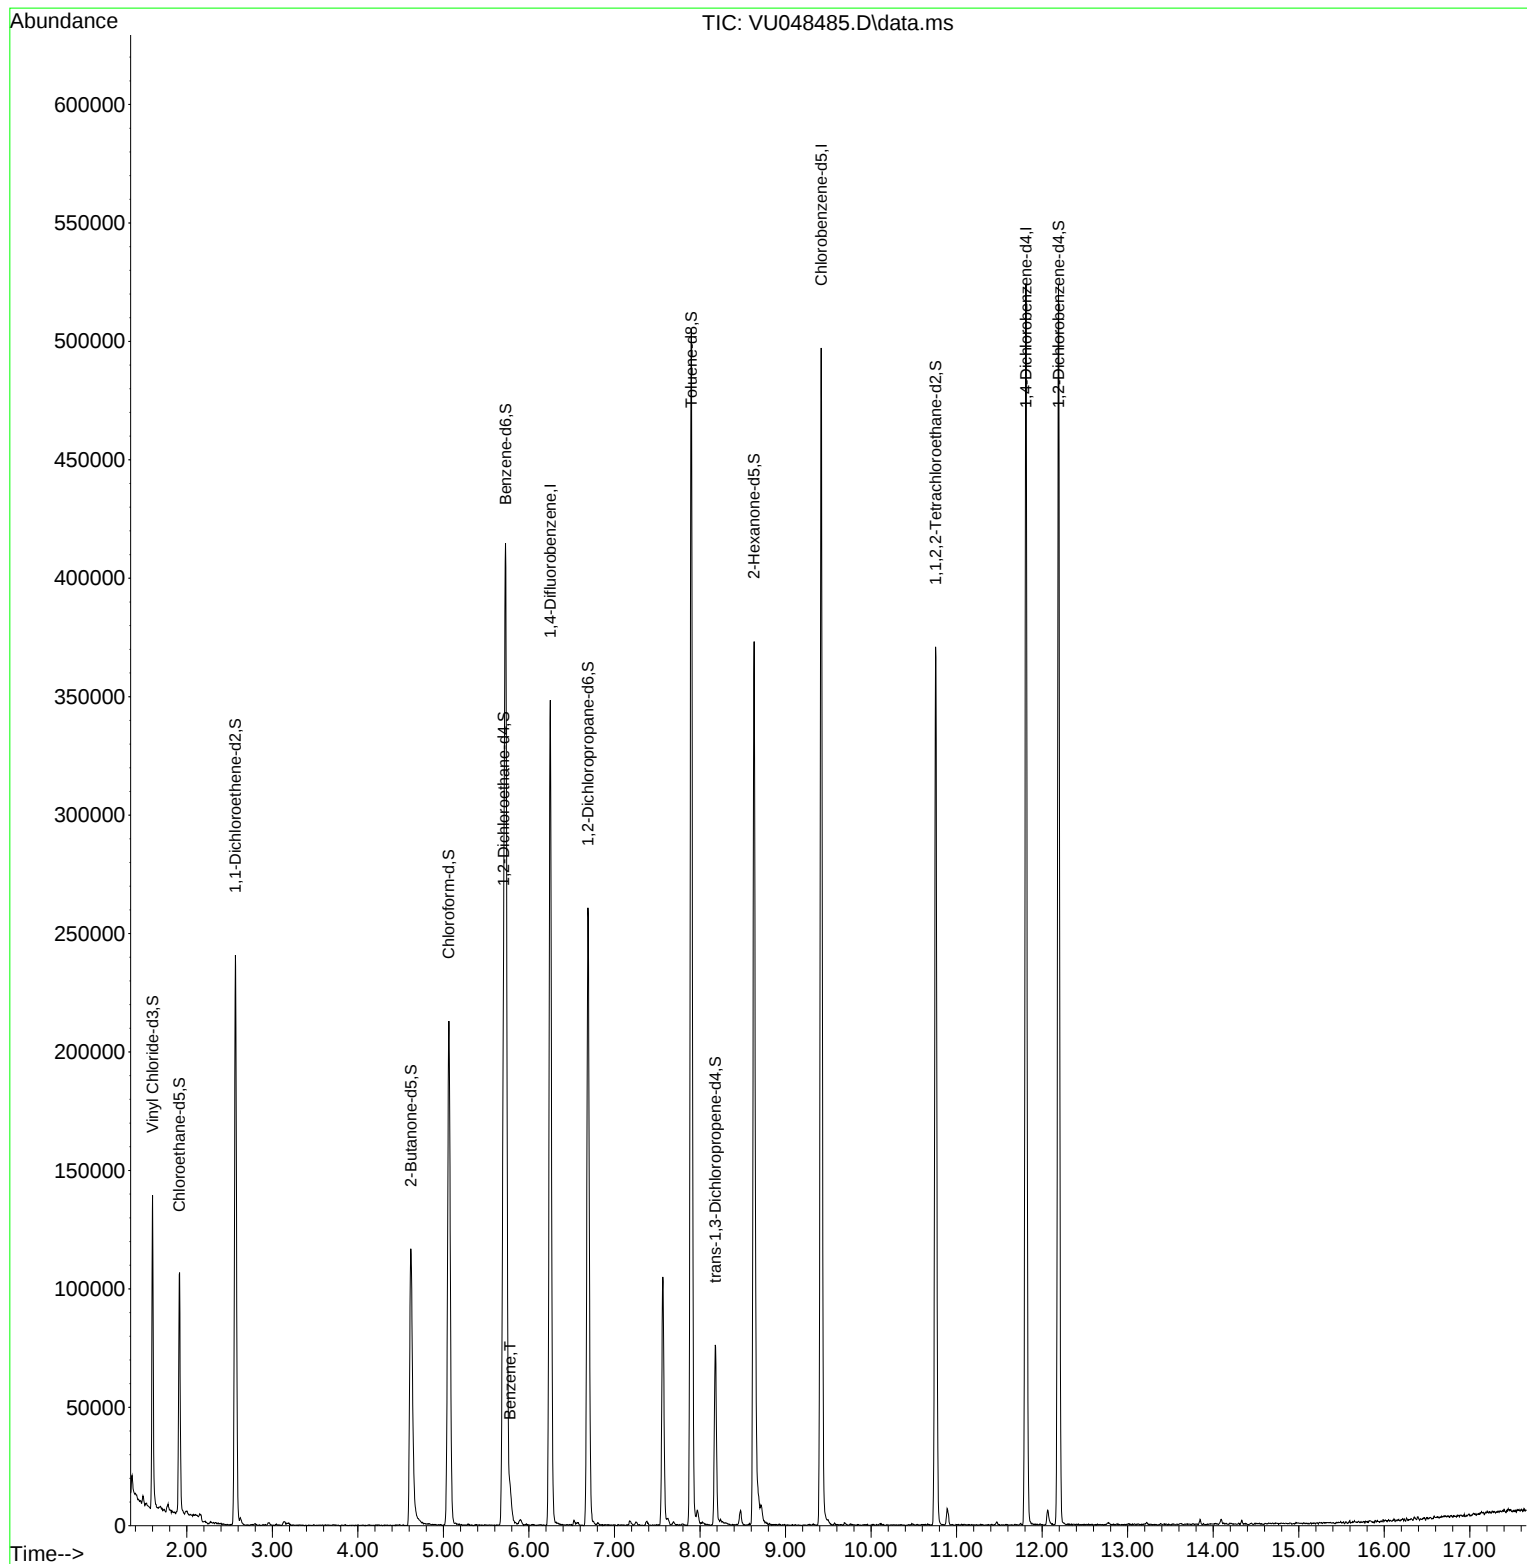

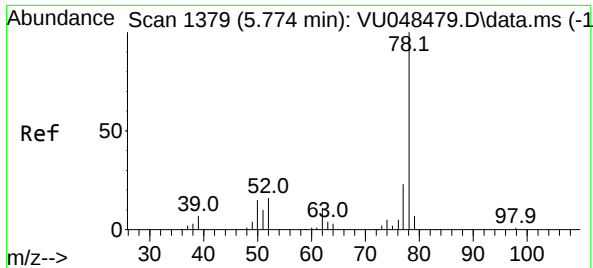

#33
Benzene
Concen: 1.276 ug/L
RT: 5.777 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU048485.D
Acq: 10 May 2022 12:54

Instrument :
MSVOA_U
ClientSampleId :
EXEW1

Tgt Ion: 78 Resp: 12175

