

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048495.D
 Acq On : 10 May 2022 16:47
 Operator : SY/MD
 Sample : VIBLK070
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK070

Quant Time: May 11 05:23:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 05:17:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	263294	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	260470	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	129253	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	80927	35.689	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.380%
7) Chloroethane-d5	1.912	69	64190	43.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.760%
11) 1,1-Dichloroethene-d2	2.568	63	134634	33.362	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.720%
21) 2-Butanone-d5	4.623	46	162184	83.984	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.980%
24) Chloroform-d	5.063	84	191432	48.605	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.703	65	136726	53.404	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.800%
32) Benzene-d6	5.729	84	356312	45.016	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.040%
36) 1,2-Dichloropropane-d6	6.690	67	112095	43.429	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.860%
41) Toluene-d8	7.899	98	314448	44.919	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.840%
43) trans-1,3-Dichloroprop...	8.179	79	41302	34.766	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.540%
47) 2-Hexanone-d5	8.632	63	121372	97.154	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.150%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	166534	42.358	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.720%
66) 1,2-Dichlorobenzene-d4	12.192	152	129315	50.525	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.060%
Target Compounds						
13) Acetone	2.629	43	17131	11.767	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048495.D
Acq On : 10 May 2022 16:47
Operator : SY/MD
Sample : VIBLK070
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK070

Quant Time: May 11 05:23:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 05:17:27 2022
Response via : Initial Calibration

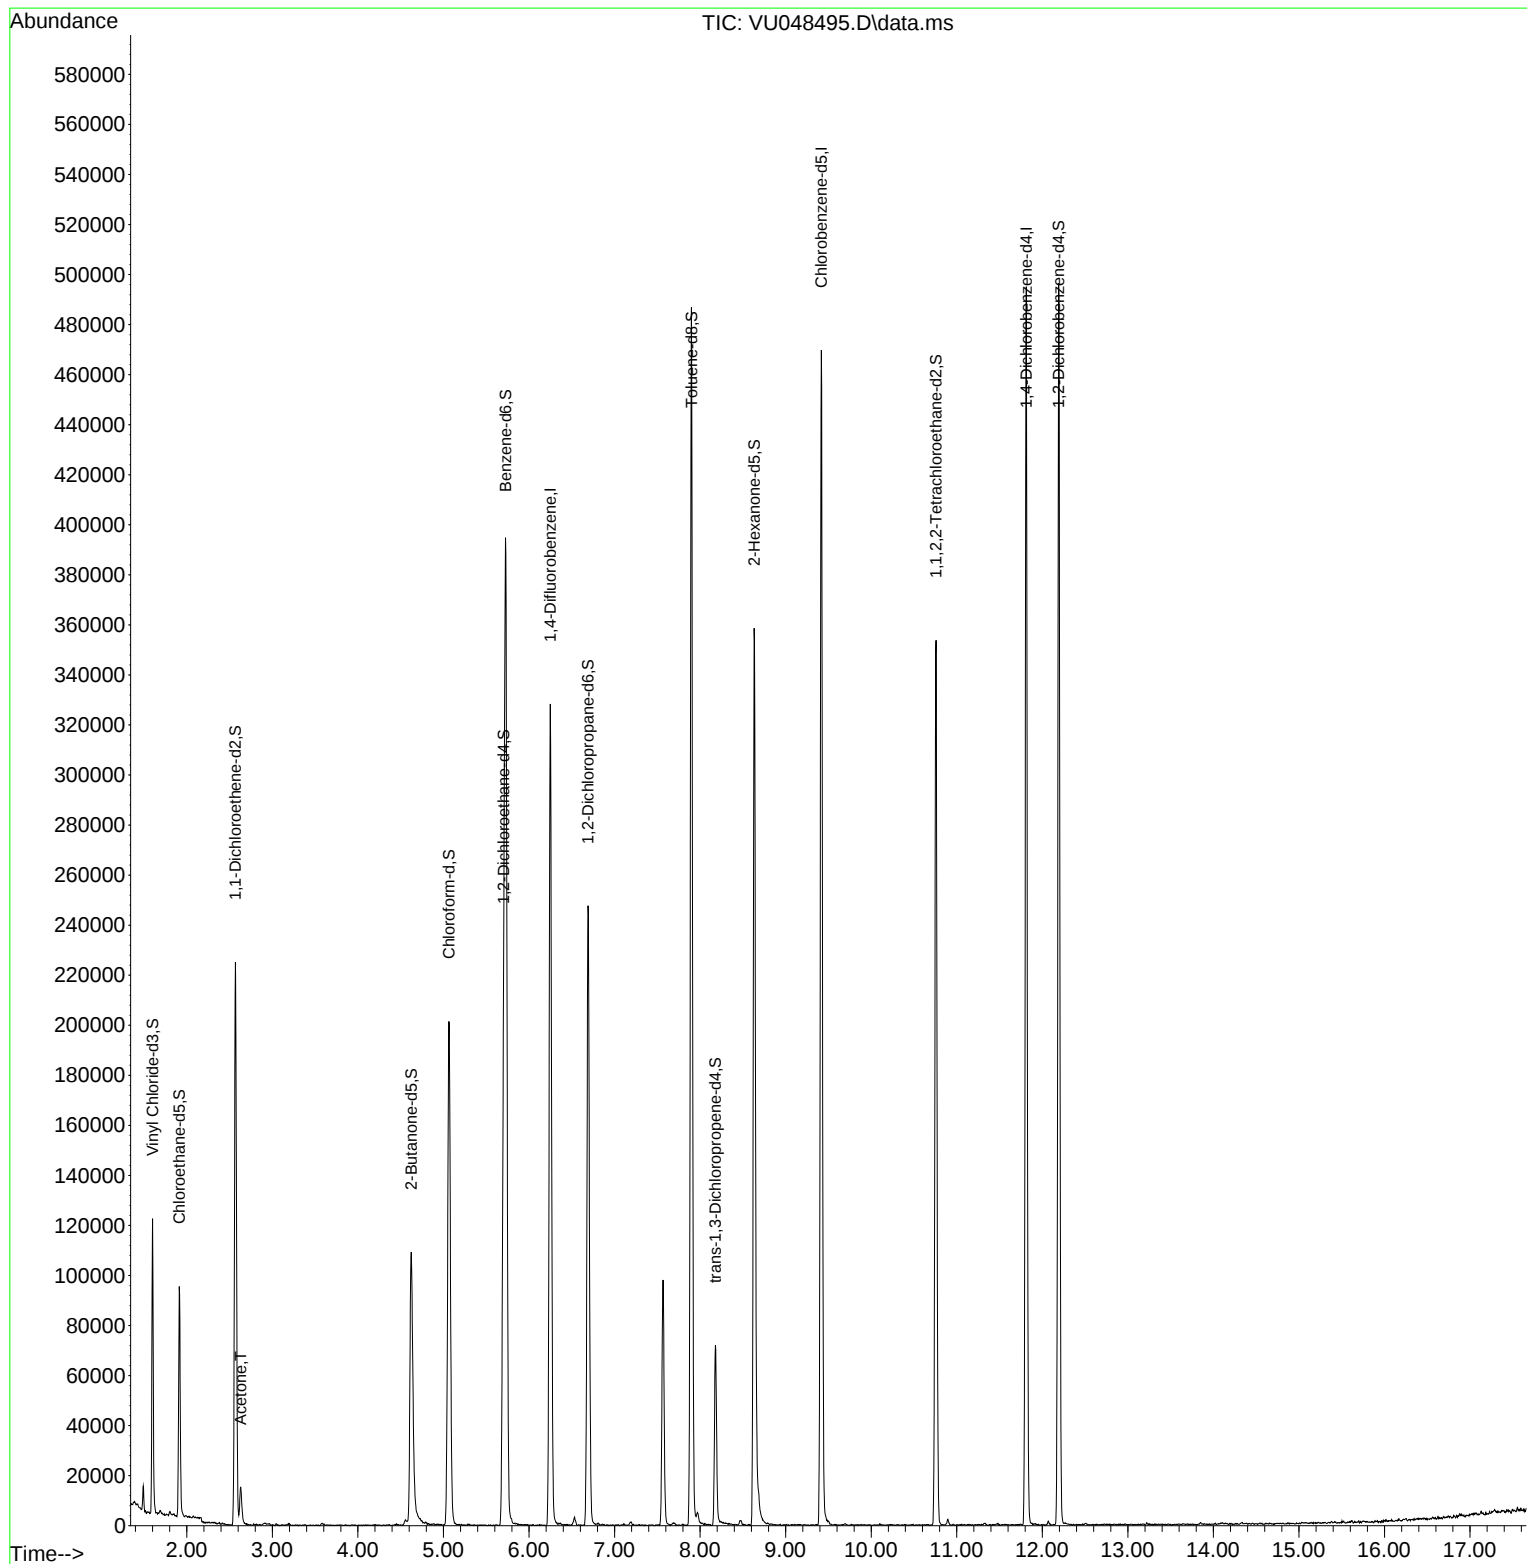

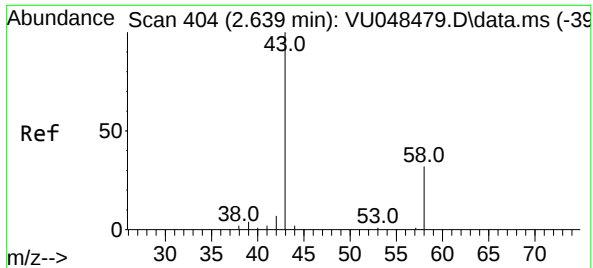

#13
 Acetone
 Concen: 11.767 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. -0.010 min
 Lab File: VU048495.D
 Acq: 10 May 2022 16:47

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK070

Tgt Ion: 43 Resp: 17131
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 66.2

