

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048485.D
 Acq On : 10 May 2022 12:54
 Operator : SY/MD
 Sample : N2736-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	102	rVB	132092	148036	12.68%	1.685%
2	1.916	171	179	197	rVB	101973	133448	11.43%	1.519%
3	2.568	370	382	397	rBV	240405	390644	33.47%	4.446%
4	2.713	425	427	432	rVB2	301	183	0.02%	0.002%
5	2.755	435	440	441	rBV	299	275	0.02%	0.003%
6	2.893	480	483	487	rVB2	362	207	0.02%	0.002%
7	2.916	488	490	494	rBV2	372	216	0.02%	0.002%
8	3.038	524	528	529	rBV	465	264	0.02%	0.003%
9	3.076	538	540	545	rVB2	291	192	0.02%	0.002%
10	3.137	550	559	560	rBV2	1600	1866	0.16%	0.021%
11	3.244	590	592	597	rVV2	242	198	0.02%	0.002%
12	3.321	610	616	620	rBV2	258	358	0.03%	0.004%
13	3.391	634	638	644	rBV	263	331	0.03%	0.004%
14	3.481	663	666	667	rBV	241	131	0.01%	0.001%
15	3.588	695	699	702	rBV2	236	186	0.02%	0.002%
16	3.642	713	716	718	rBV	211	124	0.01%	0.001%
17	3.710	733	737	740	rBV	262	282	0.02%	0.003%
18	3.813	767	769	775	rVB	227	176	0.02%	0.002%
19	3.842	775	778	779	rBV	185	132	0.01%	0.002%
20	3.973	816	819	822	rBV	259	223	0.02%	0.003%
21	4.002	826	828	832	rVV	261	167	0.01%	0.002%
22	4.211	890	893	896	rBV	213	141	0.01%	0.002%
23	4.276	911	913	917	rVB	314	218	0.02%	0.002%
24	4.301	917	921	923	rBV	194	174	0.01%	0.002%
25	4.314	923	925	929	rVV2	204	161	0.01%	0.002%
26	4.350	934	936	941	rVV	186	148	0.01%	0.002%
27	4.379	942	945	948	rVB2	190	150	0.01%	0.002%
28	4.488	977	979	984	rVB	352	216	0.02%	0.002%
29	4.620	1007	1020	1059	rBV	116806	290220	24.86%	3.303%
30	5.009	1138	1141	1142	rBV	314	169	0.01%	0.002%
31	5.063	1142	1158	1179	rVV	212698	463122	39.68%	5.271%
32	5.189	1194	1197	1200	rVB2	507	308	0.03%	0.004%
33	5.211	1200	1204	1205	rVV2	343	223	0.02%	0.003%
34	5.237	1209	1212	1215	rBV2	242	215	0.02%	0.002%
35	5.288	1224	1228	1232	rBV4	576	482	0.04%	0.005%
36	5.343	1243	1245	1249	rVB	276	194	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048485.D
 Acq On : 10 May 2022 12:54
 Operator : SY/MD
 Sample : N2736-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.369	1249	1253	1255	rBV2	394	327	0.03%	0.004%
38	5.485	1286	1289	1291	rBV	308	223	0.02%	0.003%
39	5.626	1330	1333	1335	rBV2	286	135	0.01%	0.002%
40	5.726	1340	1364	1398	rBV2	414628	1167268	100.00%	13.285%
41	5.948	1430	1433	1434	rBV	286	170	0.01%	0.002%
42	5.970	1438	1440	1443	rVB3	617	366	0.03%	0.004%
43	6.028	1455	1458	1460	rBV	294	180	0.02%	0.002%
44	6.105	1477	1482	1484	rBV	274	196	0.02%	0.002%
45	6.166	1498	1501	1504	rBV2	311	208	0.02%	0.002%
46	6.250	1511	1527	1545	rBV	348444	660468	56.58%	7.517%
47	6.526	1607	1613	1619	rBV3	2197	2808	0.24%	0.032%
48	6.626	1641	1644	1648	rVB	303	252	0.02%	0.003%
49	6.690	1649	1664	1682	rBV	260887	503033	43.09%	5.725%
50	6.867	1718	1719	1721	rBV	346	151	0.01%	0.002%
51	6.935	1737	1740	1744	rVB2	302	228	0.02%	0.003%
52	6.957	1745	1747	1749	rBV	193	129	0.01%	0.001%
53	7.044	1771	1774	1779	rBV2	421	407	0.03%	0.005%
54	7.083	1783	1786	1788	rVV	216	130	0.01%	0.001%
55	7.095	1788	1790	1794	rVB2	193	118	0.01%	0.001%
56	7.144	1802	1805	1807	rBV	251	131	0.01%	0.001%
57	7.179	1811	1816	1829	rVB5	1912	3333	0.29%	0.038%
58	7.253	1829	1839	1846	rBV7	1435	2609	0.22%	0.030%
59	7.378	1871	1878	1881	rBV5	1652	2155	0.18%	0.025%
60	7.449	1895	1900	1904	rBV2	266	235	0.02%	0.003%
61	7.468	1904	1906	1910	rBV2	181	148	0.01%	0.002%
62	7.565	1924	1936	1950	rBV	104825	183868	15.75%	2.093%
63	7.735	1986	1989	1994	rVB3	377	322	0.03%	0.004%
64	7.793	2003	2007	2009	rBV2	483	428	0.04%	0.005%
65	7.899	2025	2040	2057	rBV	505099	884778	75.80%	10.070%
66	8.179	2116	2127	2143	rBV2	75852	129615	11.10%	1.475%
67	8.382	2188	2190	2194	rVB	281	149	0.01%	0.002%
68	8.632	2256	2268	2289	rBV	372553	664235	56.91%	7.560%
69	8.816	2321	2325	2327	rBV3	550	387	0.03%	0.004%
70	8.970	2370	2373	2377	rBV2	254	220	0.02%	0.003%
71	9.076	2404	2406	2408	rBV2	294	130	0.01%	0.001%
72	9.115	2413	2418	2421	rBV2	313	274	0.02%	0.003%
73	9.417	2498	2512	2534	rBV	497034	834713	71.51%	9.500%
74	9.562	2555	2557	2558	rBV	442	202	0.02%	0.002%
75	9.687	2591	2596	2604	rBV2	1185	1678	0.14%	0.019%
76	9.755	2614	2617	2619	rBV	495	346	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048485.D
 Acq On : 10 May 2022 12:54
 Operator : SY/MD
 Sample : N2736-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.848	2644	2646	2650	rBV2	326	216	0.02%	0.002%
78	9.922	2667	2669	2673	rBV	241	145	0.01%	0.002%
79	10.012	2694	2697	2698	rBV	344	132	0.01%	0.002%
80	10.346	2799	2801	2806	rBV2	304	300	0.03%	0.003%
81	10.475	2839	2841	2842	rBV	344	108	0.01%	0.001%
82	10.639	2890	2892	2896	rBV	336	203	0.02%	0.002%
83	10.661	2897	2899	2902	rVV2	433	214	0.02%	0.002%
84	10.754	2915	2928	2952	rBV	370867	601158	51.50%	6.842%
85	10.890	2961	2970	2981	rBV3	6972	11439	0.98%	0.130%
86	10.992	3000	3002	3005	rBV2	273	143	0.01%	0.002%
87	11.089	3028	3032	3033	rBV	409	319	0.03%	0.004%
88	11.253	3081	3083	3086	rBV	162	106	0.01%	0.001%
89	11.372	3117	3120	3124	rBV	276	176	0.02%	0.002%
90	11.571	3179	3182	3183	rBV2	317	196	0.02%	0.002%
91	11.812	3244	3257	3277	rBV	524109	838881	71.87%	9.548%
92	12.037	3325	3327	3328	rBV	271	115	0.01%	0.001%
93	12.066	3328	3336	3346	rVV6	6133	10461	0.90%	0.119%
94	12.192	3362	3375	3393	rBV	523142	837353	71.74%	9.531%
95	12.542	3482	3484	3487	rVB	361	167	0.01%	0.002%
96	12.626	3509	3510	3513	rVB	275	109	0.01%	0.001%
97	13.057	3641	3644	3646	rBV	479	268	0.02%	0.003%
98	13.111	3657	3661	3663	rBV	507	426	0.04%	0.005%
99	13.520	3785	3788	3791	rBV	397	311	0.03%	0.004%
100	13.848	3884	3890	3898	rVB4	2214	2552	0.22%	0.029%




Sum of corrected areas: 8786031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048485.D
Acq On : 10 May 2022 12:54
Operator : SY/MD
Sample : N2736-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

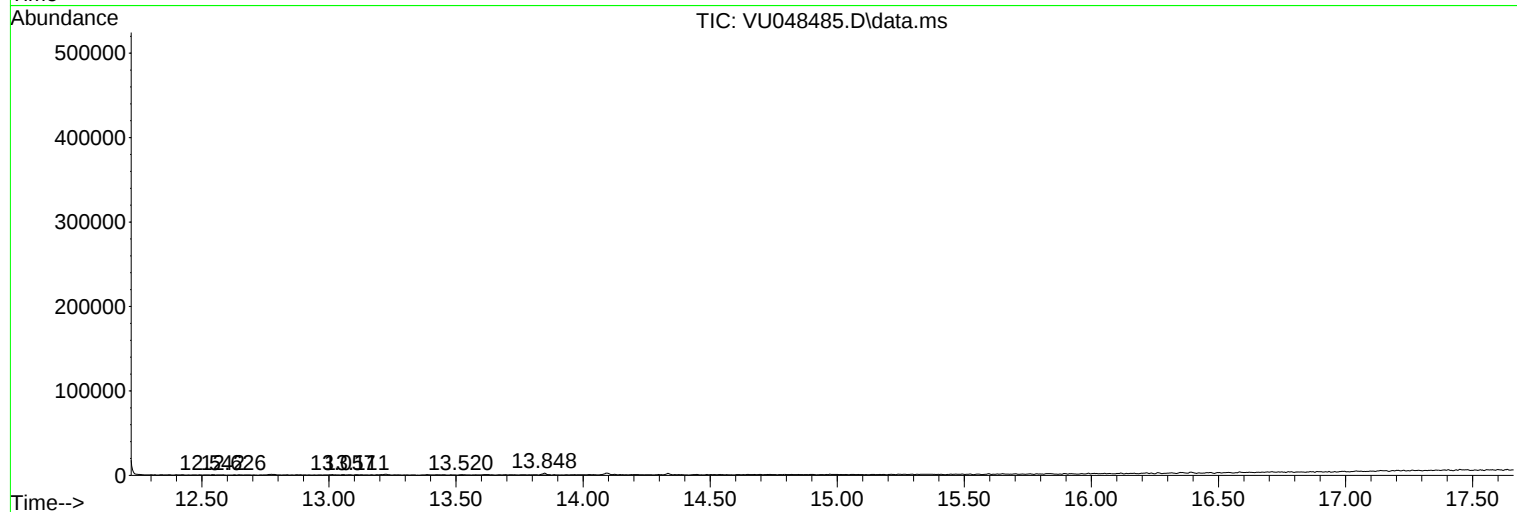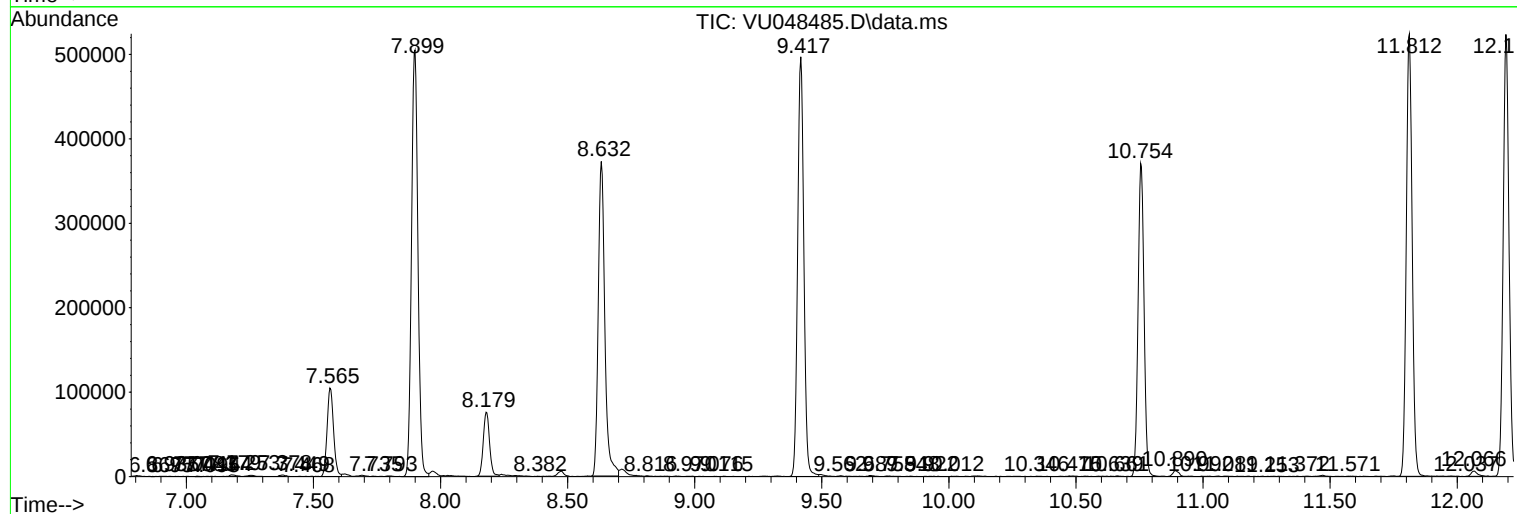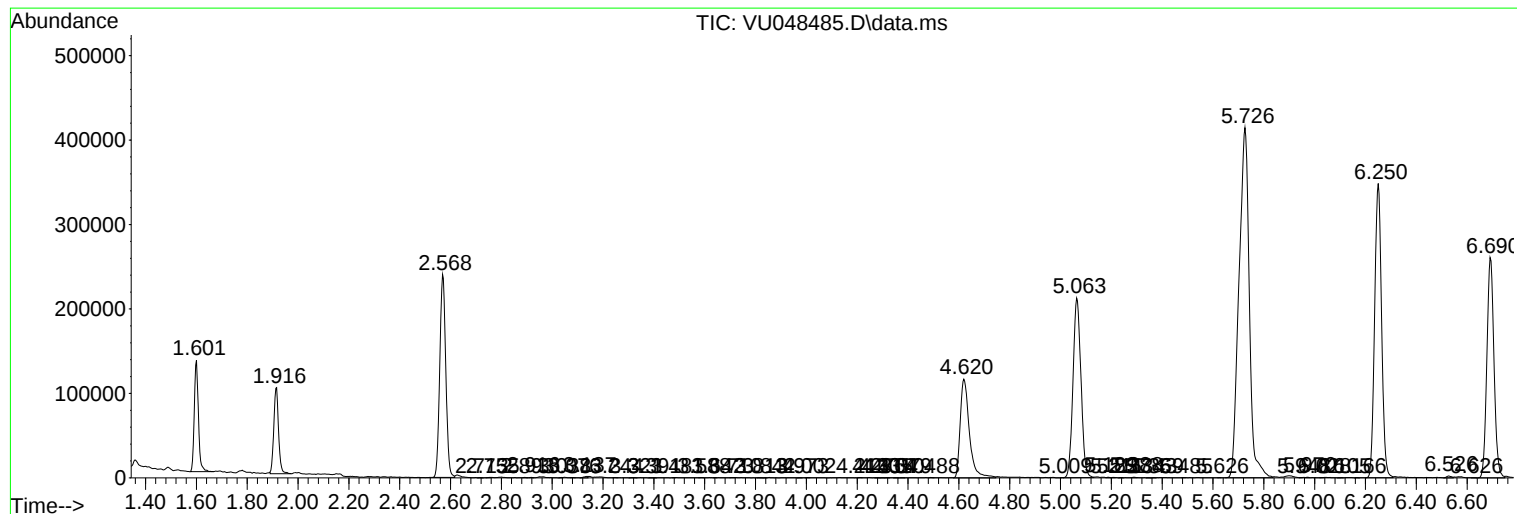

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048485.D
Acq On : 10 May 2022 12:54
Operator : SY/MD
Sample : N2736-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048485.D
Acq On : 10 May 2022 12:54
Operator : SY/MD
Sample : N2736-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc