

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048488.D
 Acq On : 10 May 2022 14:04
 Operator : SY/MD
 Sample : N2736-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	99	rVB	125810	145276	13.12%	1.718%
2	1.916	171	179	191	rBV	96040	123201	11.13%	1.457%
3	2.568	370	382	395	rBV	236666	381309	34.44%	4.508%
4	2.684	414	418	421	rBB	301	220	0.02%	0.003%
5	2.829	461	463	466	rVB	317	145	0.01%	0.002%
6	2.970	505	507	513	rVB2	462	349	0.03%	0.004%
7	3.109	549	550	554	rVB	327	162	0.01%	0.002%
8	3.131	554	557	560	rBV2	304	235	0.02%	0.003%
9	3.183	563	573	585	rVB5	1492	3472	0.31%	0.041%
10	3.285	600	605	609	rBV	297	216	0.02%	0.003%
11	3.327	611	618	623	rVB2	494	535	0.05%	0.006%
12	3.498	668	671	676	rBV	210	170	0.02%	0.002%
13	3.813	768	769	771	rBV2	370	188	0.02%	0.002%
14	3.842	776	778	784	rVB2	282	232	0.02%	0.003%
15	3.983	816	822	827	rBV	235	364	0.03%	0.004%
16	4.086	850	854	855	rBV	156	136	0.01%	0.002%
17	4.189	882	886	889	rVB	211	136	0.01%	0.002%
18	4.253	901	906	909	rVV2	210	212	0.02%	0.003%
19	4.292	913	918	919	rBV	180	149	0.01%	0.002%
20	4.301	919	921	924	rVB	282	135	0.01%	0.002%
21	4.475	973	975	981	rVB	243	159	0.01%	0.002%
22	4.533	990	993	998	rVB2	313	300	0.03%	0.004%
23	4.559	999	1001	1004	rBB	272	144	0.01%	0.002%
24	4.620	1005	1020	1046	rBV	97892	236868	21.40%	2.800%
25	4.938	1116	1119	1121	rBV	255	154	0.01%	0.002%
26	4.986	1131	1134	1136	rBV2	445	318	0.03%	0.004%
27	5.064	1141	1158	1178	rVV	206248	456505	41.24%	5.397%
28	5.250	1213	1216	1217	rBV	267	167	0.02%	0.002%
29	5.343	1243	1245	1250	rVB2	191	149	0.01%	0.002%
30	5.385	1255	1258	1261	rBV	422	227	0.02%	0.003%
31	5.411	1261	1266	1271	rVB2	262	246	0.02%	0.003%
32	5.478	1283	1287	1289	rBV	402	289	0.03%	0.003%
33	5.552	1306	1310	1314	rBV2	270	235	0.02%	0.003%
34	5.617	1326	1330	1332	rVB2	234	152	0.01%	0.002%
35	5.652	1337	1341	1342	rBV	245	156	0.01%	0.002%
36	5.726	1342	1364	1381	rBV2	404997	1107026	100.00%	13.088%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048488.D
 Acq On : 10 May 2022 14:04
 Operator : SY/MD
 Sample : N2736-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.941	1428	1431	1435	rVB	229	181	0.02%	0.002%
38	5.964	1435	1438	1443	rBV2	503	384	0.03%	0.005%
39	5.986	1443	1445	1448	rBV2	321	157	0.01%	0.002%
40	6.108	1478	1483	1485	rBV2	262	273	0.02%	0.003%
41	6.160	1495	1499	1503	rVB3	327	208	0.02%	0.002%
42	6.250	1513	1527	1558	rBV	344564	649910	58.71%	7.683%
43	6.526	1605	1613	1614	rBV4	2941	2873	0.26%	0.034%
44	6.594	1632	1634	1638	rVB	550	388	0.04%	0.005%
45	6.690	1650	1664	1684	rBV	250378	490569	44.31%	5.800%
46	6.800	1693	1698	1700	rBV2	751	731	0.07%	0.009%
47	6.909	1728	1732	1735	rBV2	266	236	0.02%	0.003%
48	6.961	1745	1748	1749	rBV	465	223	0.02%	0.003%
49	7.012	1759	1764	1767	rBV2	436	509	0.05%	0.006%
50	7.041	1769	1773	1774	rBV	263	158	0.01%	0.002%
51	7.179	1810	1816	1818	rBV2	1954	1824	0.16%	0.022%
52	7.260	1838	1841	1844	rVB	233	133	0.01%	0.002%
53	7.343	1864	1867	1869	rBV	266	166	0.01%	0.002%
54	7.462	1899	1904	1908	rBV2	311	309	0.03%	0.004%
55	7.504	1915	1917	1921	rBV	358	240	0.02%	0.003%
56	7.565	1924	1936	1949	rBV	97693	172455	15.58%	2.039%
57	7.800	2003	2009	2014	rBV3	527	601	0.05%	0.007%
58	7.899	2026	2040	2056	rBV	502787	862617	77.92%	10.198%
59	8.179	2114	2127	2146	rBV	73174	124642	11.26%	1.474%
60	8.472	2208	2218	2222	rBV3	1705	2724	0.25%	0.032%
61	8.575	2242	2250	2257	rBV3	3689	5529	0.50%	0.065%
62	8.632	2257	2268	2292	rBV	357239	636564	57.50%	7.526%
63	8.832	2326	2330	2333	rBV2	414	277	0.03%	0.003%
64	8.851	2333	2336	2338	rBV	341	188	0.02%	0.002%
65	8.957	2364	2369	2373	rBV2	472	452	0.04%	0.005%
66	9.112	2413	2417	2420	rBV2	370	267	0.02%	0.003%
67	9.160	2430	2432	2434	rBV	260	153	0.01%	0.002%
68	9.304	2473	2477	2481	rBV2	328	327	0.03%	0.004%
69	9.372	2496	2498	2499	rBV	277	142	0.01%	0.002%
70	9.417	2499	2512	2534	rVV	491921	820998	74.16%	9.706%
71	9.642	2579	2582	2586	rBV2	272	227	0.02%	0.003%
72	9.848	2642	2646	2647	rBV	352	257	0.02%	0.003%
73	9.922	2665	2669	2673	rBV2	235	189	0.02%	0.002%
74	9.976	2683	2686	2688	rBV	366	286	0.03%	0.003%
75	10.038	2701	2705	2711	rBV2	331	318	0.03%	0.004%
76	10.073	2712	2716	2720	rBV2	287	268	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048488.D
 Acq On : 10 May 2022 14:04
 Operator : SY/MD
 Sample : N2736-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.099	2720	2724	2727	rBV3	452	341	0.03%	0.004%
78	10.115	2727	2729	2731	rBV	215	136	0.01%	0.002%
79	10.163	2741	2744	2747	rBV	251	220	0.02%	0.003%
80	10.427	2824	2826	2828	rBV	293	162	0.01%	0.002%
81	10.485	2843	2844	2850	rVB2	653	339	0.03%	0.004%
82	10.555	2864	2866	2873	rVB	414	203	0.02%	0.002%
83	10.587	2874	2876	2878	rBV	222	132	0.01%	0.002%
84	10.755	2916	2928	2948	rBV	364703	589986	53.29%	6.975%
85	11.237	3075	3078	3080	rBV	457	247	0.02%	0.003%
86	11.517	3161	3165	3168	rBV	329	255	0.02%	0.003%
87	11.539	3169	3172	3175	rBV2	251	223	0.02%	0.003%
88	11.738	3231	3234	3235	rBV	540	326	0.03%	0.004%
89	11.812	3244	3257	3273	rBV	519487	810969	73.26%	9.588%
90	12.038	3325	3327	3329	rVB	509	167	0.02%	0.002%
91	12.128	3353	3355	3357	rBV	369	194	0.02%	0.002%
92	12.192	3363	3375	3393	rBV	497242	812960	73.44%	9.611%
93	12.404	3439	3441	3444	rVB	424	153	0.01%	0.002%
94	12.796	3560	3563	3565	rBV2	448	249	0.02%	0.003%
95	13.018	3629	3632	3639	rVB3	573	538	0.05%	0.006%
96	13.221	3692	3695	3698	rBV2	875	650	0.06%	0.008%
97	13.295	3715	3718	3721	rBV2	303	167	0.02%	0.002%
98	13.970	3923	3928	3932	rBV	568	539	0.05%	0.006%
99	14.301	4029	4031	4034	rBV2	550	188	0.02%	0.002%
100	15.475	4394	4396	4399	rBV2	898	339	0.03%	0.004%




Sum of corrected areas: 8458573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048488.D
Acq On : 10 May 2022 14:04
Operator : SY/MD
Sample : N2736-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

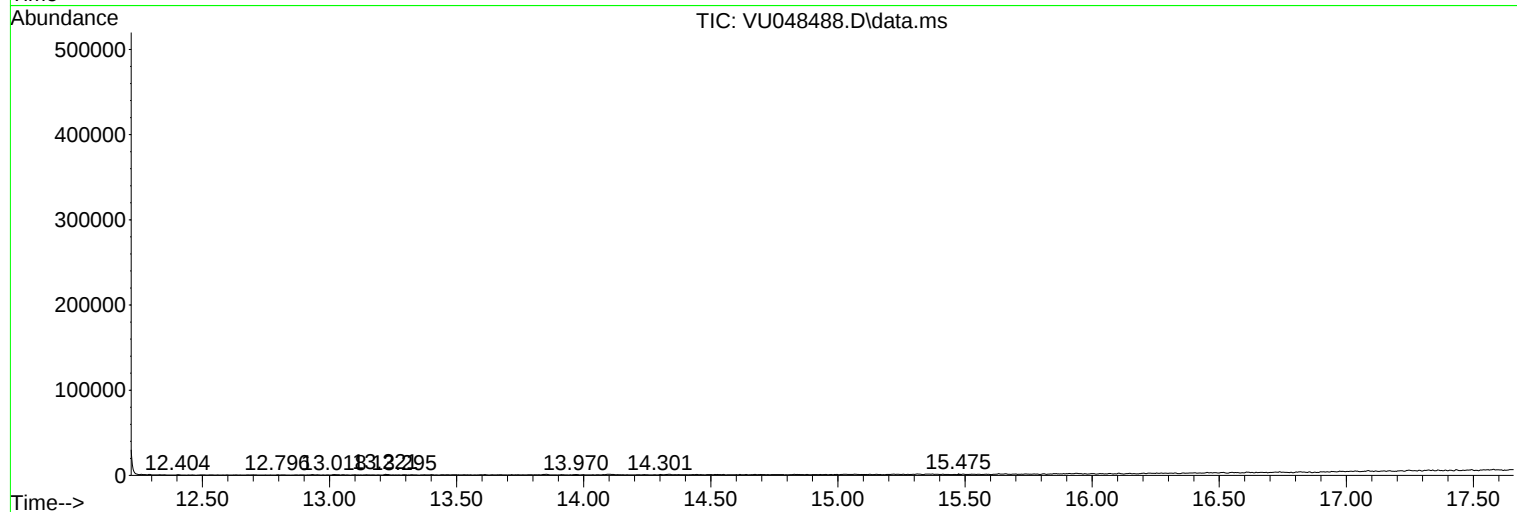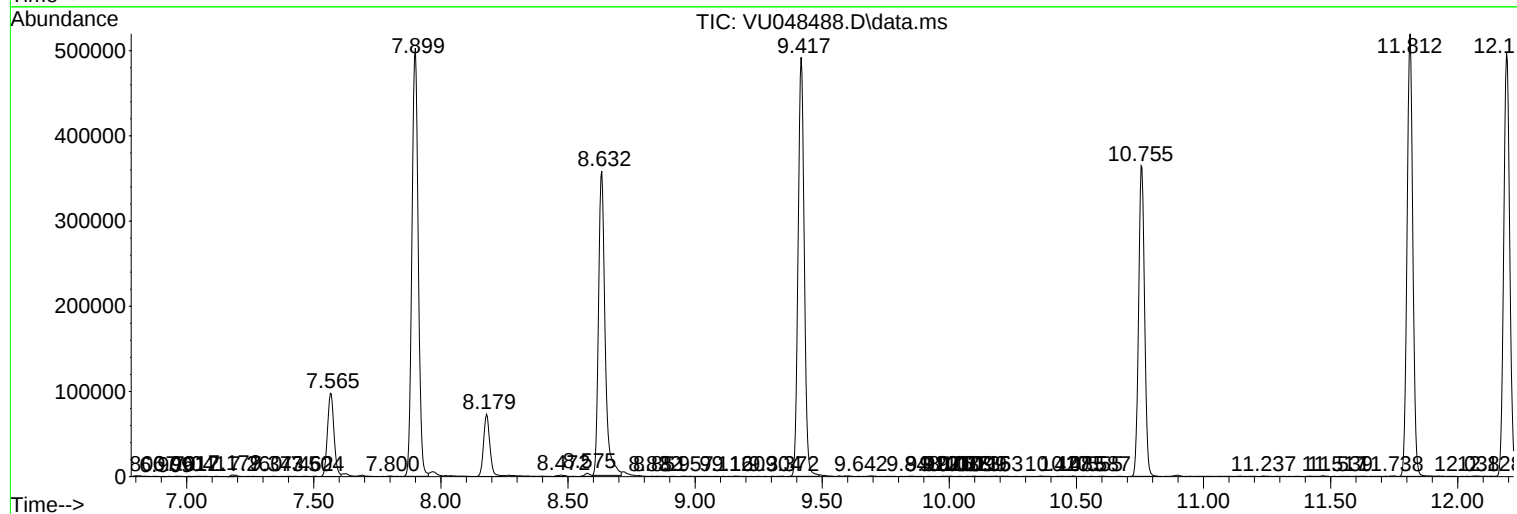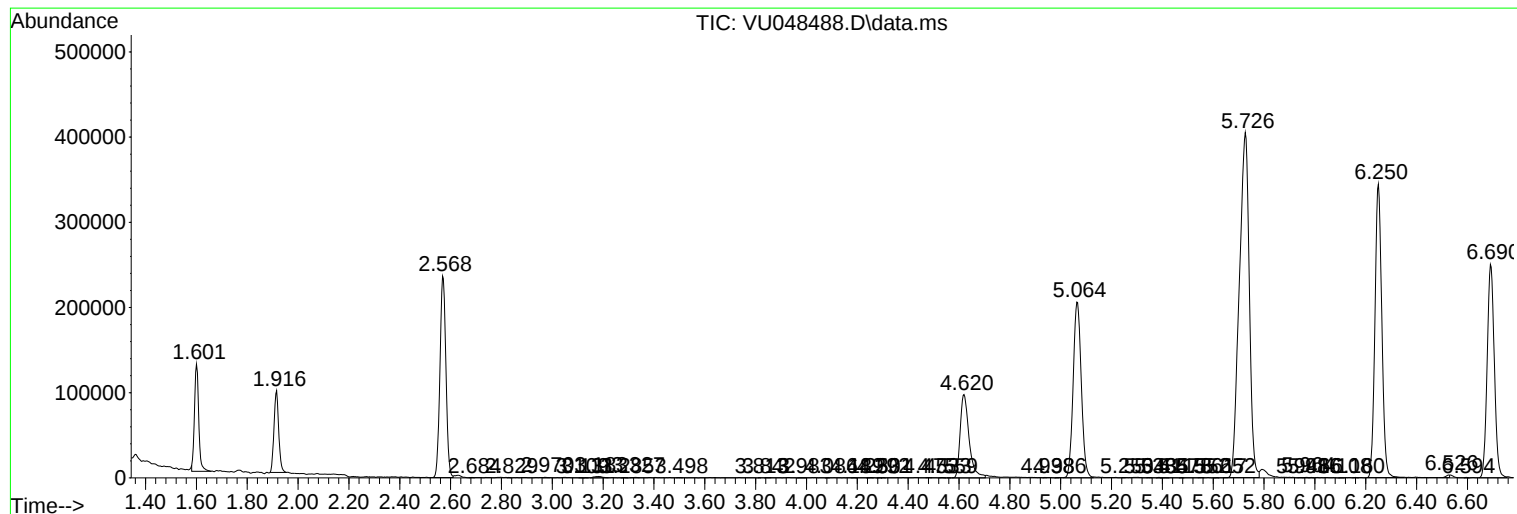

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048488.D
Acq On : 10 May 2022 14:04
Operator : SY/MD
Sample : N2736-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048488.D
Acq On : 10 May 2022 14:04
Operator : SY/MD
Sample : N2736-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------