

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048498.D
 Acq On : 10 May 2022 17:57
 Operator : SY/MD
 Sample : N2710-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M

Title : VOC Analysis

Signal : TIC: VU048498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	113625	128565	12.25%	1.523%
2	1.913	171	178	193	rVB	88286	115759	11.03%	1.371%
3	2.240	277	280	285	rBV3	897	877	0.08%	0.010%
4	2.286	291	294	295	rBV2	657	395	0.04%	0.005%
5	2.568	369	382	398	rBV	219816	357913	34.11%	4.239%
6	2.710	420	426	431	rBV2	287	407	0.04%	0.005%
7	2.887	478	481	484	rBV2	243	167	0.02%	0.002%
8	2.951	499	501	504	rBV2	348	147	0.01%	0.002%
9	3.051	522	532	542	rVB3	4951	8838	0.84%	0.105%
10	3.089	542	544	547	rVB	275	156	0.01%	0.002%
11	3.121	548	554	555	rBV2	386	341	0.03%	0.004%
12	3.189	562	575	591	rVB	7026	15120	1.44%	0.179%
13	3.250	591	594	597	rBV	153	113	0.01%	0.001%
14	3.343	621	623	625	rBV	149	107	0.01%	0.001%
15	3.433	649	651	652	rBV	187	98	0.01%	0.001%
16	3.491	663	669	673	rVB2	377	540	0.05%	0.006%
17	3.514	673	676	679	rBV	303	284	0.03%	0.003%
18	3.578	695	696	697	rVB	114	22	0.00%	0.000%
19	3.617	704	708	711	rBV2	170	186	0.02%	0.002%
20	3.658	716	721	722	rBV	211	184	0.02%	0.002%
21	3.784	758	760	762	rBV	224	146	0.01%	0.002%
22	3.803	763	766	768	rVV	232	124	0.01%	0.001%
23	3.816	768	770	774	rVV	180	163	0.02%	0.002%
24	3.858	781	783	784	rBV	208	93	0.01%	0.001%
25	3.932	799	806	809	rBV2	310	498	0.05%	0.006%
26	4.015	830	832	833	rBB	84	46	0.00%	0.001%
27	4.183	881	884	889	rVB2	206	183	0.02%	0.002%
28	4.253	903	906	909	rBV2	445	352	0.03%	0.004%
29	4.308	921	923	925	rBV2	165	69	0.01%	0.001%
30	4.350	931	936	940	rBV2	372	393	0.04%	0.005%
31	4.372	940	943	949	rVB2	281	307	0.03%	0.004%
32	4.411	953	955	958	rBV	349	245	0.02%	0.003%
33	4.433	958	962	965	rBV	238	178	0.02%	0.002%
34	4.478	975	976	977	rBV	107	41	0.00%	0.000%
35	4.501	981	983	989	rVB2	237	261	0.02%	0.003%
36	4.620	1007	1020	1042	rBV	122175	289895	27.63%	3.433%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048498.D
 Acq On : 10 May 2022 17:57
 Operator : SY/MD
 Sample : N2710-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	4.810	1077	1079	1081	rBV	535	194	0.02%	0.002%
38	5.064	1142	1158	1179	rBV	202758	443144	42.23%	5.248%
39	5.282	1223	1226	1229	rBV3	374	181	0.02%	0.002%
40	5.417	1264	1268	1271	rBV	295	260	0.02%	0.003%
41	5.446	1275	1277	1284	rVB2	302	210	0.02%	0.002%
42	5.488	1284	1290	1293	rBV2	206	243	0.02%	0.003%
43	5.539	1304	1306	1307	rBV	210	88	0.01%	0.001%
44	5.600	1323	1325	1328	rVB	213	94	0.01%	0.001%
45	5.642	1335	1338	1341	rBV2	193	147	0.01%	0.002%
46	5.726	1341	1364	1397	rBV2	376263	1049303	100.00%	12.428%
47	5.880	1407	1412	1416	rBV4	640	828	0.08%	0.010%
48	6.022	1452	1456	1457	rBV2	285	163	0.02%	0.002%
49	6.060	1466	1468	1473	rBV	291	257	0.02%	0.003%
50	6.109	1476	1483	1486	rBV3	350	383	0.04%	0.005%
51	6.125	1486	1488	1491	rVB	465	208	0.02%	0.002%
52	6.166	1493	1501	1503	rBV2	315	315	0.03%	0.004%
53	6.189	1503	1508	1510	rBV	239	192	0.02%	0.002%
54	6.250	1513	1527	1547	rBV	342711	642747	61.25%	7.613%
55	6.527	1606	1613	1623	rVB6	2285	4277	0.41%	0.051%
56	6.617	1639	1641	1642	rBV	284	98	0.01%	0.001%
57	6.690	1649	1664	1685	rBV	244097	475753	45.34%	5.635%
58	6.806	1697	1700	1708	rVB4	624	756	0.07%	0.009%
59	6.896	1725	1728	1730	rBV	277	133	0.01%	0.002%
60	6.986	1753	1756	1757	rBV	203	125	0.01%	0.001%
61	7.186	1811	1818	1826	rBV4	1700	2946	0.28%	0.035%
62	7.237	1833	1834	1837	rBV	111	35	0.00%	0.000%
63	7.256	1837	1840	1845	rBV	259	269	0.03%	0.003%
64	7.350	1866	1869	1873	rBV2	229	160	0.02%	0.002%
65	7.453	1899	1901	1904	rBV	167	136	0.01%	0.002%
66	7.520	1917	1922	1924	rBV	347	311	0.03%	0.004%
67	7.565	1924	1936	1954	rVV	131389	234070	22.31%	2.772%
68	7.748	1989	1993	1994	rBV	213	144	0.01%	0.002%
69	7.784	2001	2004	2006	rBV3	485	330	0.03%	0.004%
70	7.899	2025	2040	2056	rBV	462228	802353	76.47%	9.503%
71	8.179	2113	2127	2143	rBV	98649	165823	15.80%	1.964%
72	8.552	2240	2243	2244	rBV	267	176	0.02%	0.002%
73	8.633	2256	2268	2302	rBV	358828	648736	61.83%	7.683%
74	8.832	2327	2330	2333	rBV	417	316	0.03%	0.004%
75	8.915	2351	2356	2358	rBV3	658	614	0.06%	0.007%
76	8.973	2368	2374	2379	rBV3	392	479	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048498.D
 Acq On : 10 May 2022 17:57
 Operator : SY/MD
 Sample : N2710-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.015	2384	2387	2391	rBV	273	245	0.02%	0.003%
78	9.137	2423	2425	2427	rBV	329	98	0.01%	0.001%
79	9.340	2485	2488	2492	rBV	436	389	0.04%	0.005%
80	9.417	2499	2512	2544	rBV	488200	811603	77.35%	9.612%
81	9.671	2589	2591	2593	rBV	410	206	0.02%	0.002%
82	9.771	2620	2622	2626	rBV	411	279	0.03%	0.003%
83	9.813	2633	2635	2638	rBV2	399	204	0.02%	0.002%
84	10.095	2720	2723	2727	rBV2	528	392	0.04%	0.005%
85	10.128	2732	2733	2734	rBV	205	53	0.01%	0.001%
86	10.218	2757	2761	2764	rBV	355	293	0.03%	0.003%
87	10.430	2822	2827	2832	rVB	350	363	0.03%	0.004%
88	10.456	2832	2835	2837	rBV	363	256	0.02%	0.003%
89	10.485	2842	2844	2845	rBV	187	74	0.01%	0.001%
90	10.668	2896	2901	2908	rBV6	848	1115	0.11%	0.013%
91	10.755	2915	2928	2947	rBV	363939	586691	55.91%	6.949%
92	10.896	2965	2972	2982	rBV5	1371	2216	0.21%	0.026%
93	11.009	3004	3007	3009	rBV	169	76	0.01%	0.001%
94	11.565	3177	3180	3183	rVB	443	239	0.02%	0.003%
95	11.812	3242	3257	3278	rBV	527179	832674	79.35%	9.862%
96	11.957	3300	3302	3305	rBV2	568	485	0.05%	0.006%
97	12.192	3363	3375	3393	rBV	499688	803700	76.59%	9.519%
98	13.189	3682	3685	3690	rBV2	429	381	0.04%	0.005%
99	13.693	3839	3842	3849	rVB2	437	402	0.04%	0.005%
100	14.246	4011	4014	4019	rBV	697	626	0.06%	0.007%




Sum of corrected areas: 8443270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048498.D
Acq On : 10 May 2022 17:57
Operator : SY/MD
Sample : N2710-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

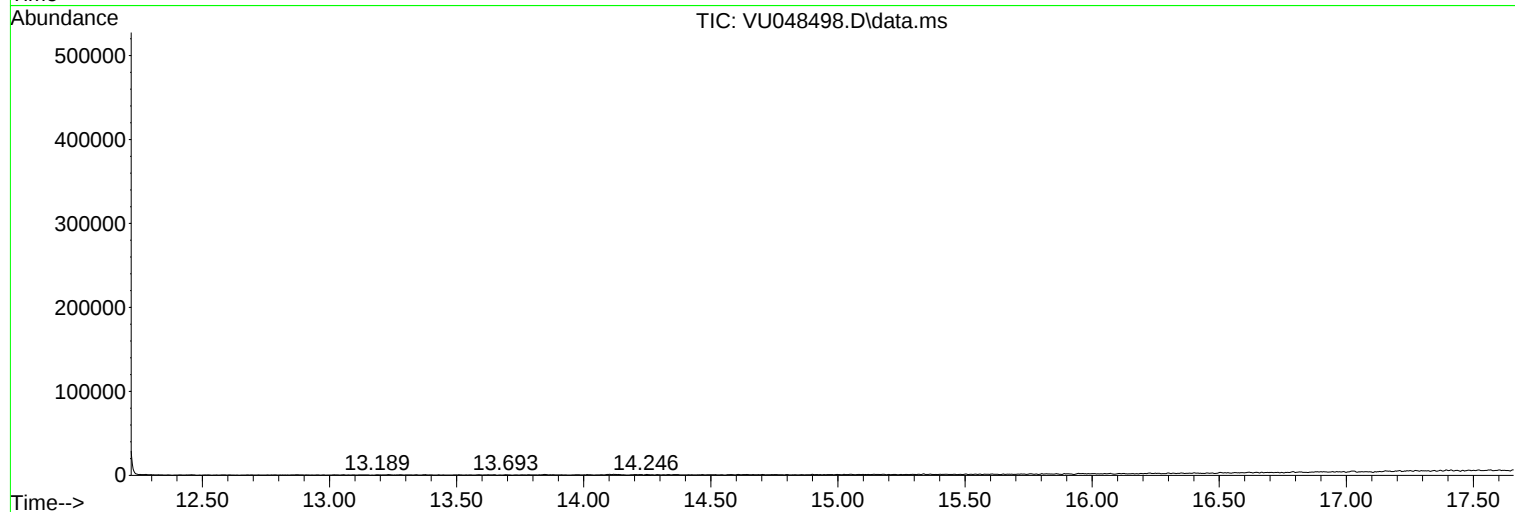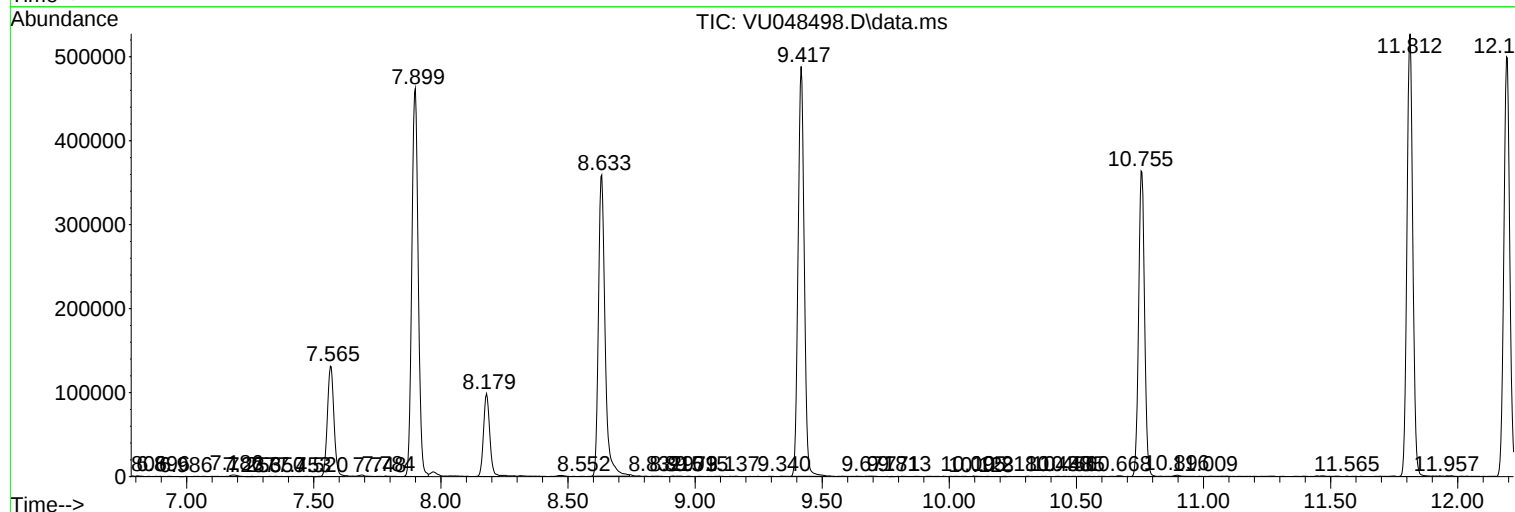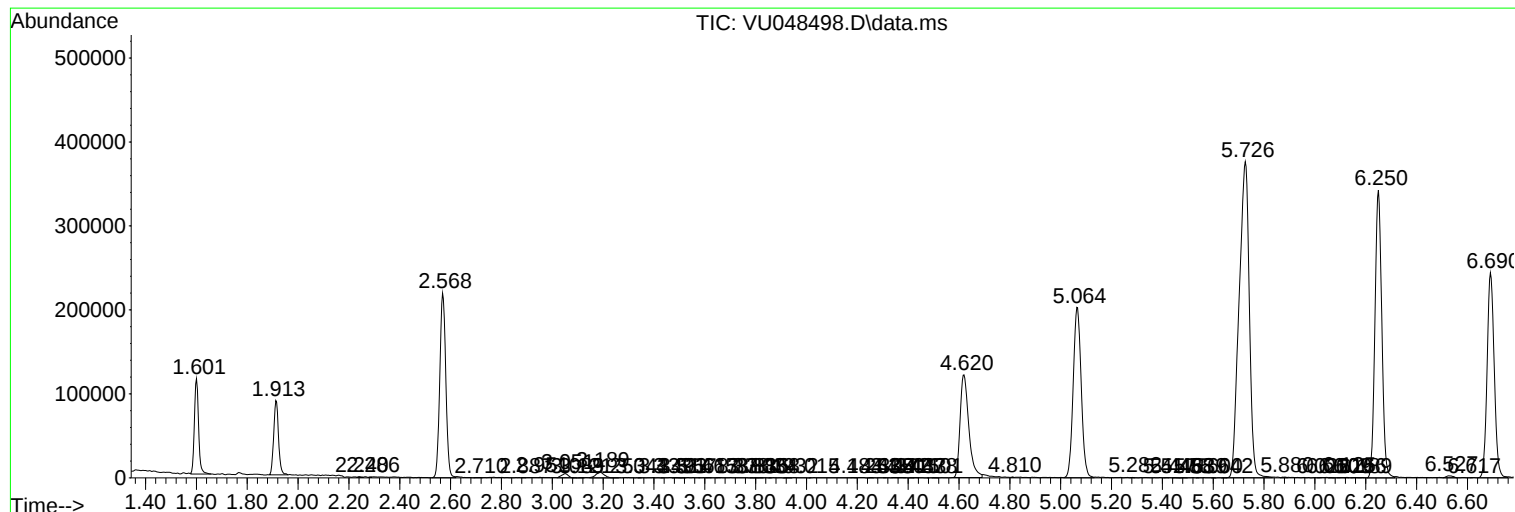

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048498.D
Acq On : 10 May 2022 17:57
Operator : SY/MD
Sample : N2710-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048498.D
Acq On : 10 May 2022 17:57
Operator : SY/MD
Sample : N2710-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc