

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048499.D
 Acq On : 10 May 2022 18:21
 Operator : SY/MD
 Sample : N2736-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rVB	109189	123574	12.08%	1.504%
2	1.912	171	178	194	rVB	87169	115538	11.29%	1.406%
3	2.568	370	382	398	rBV	209998	343914	33.61%	4.185%
4	2.674	412	415	418	rBV2	254	187	0.02%	0.002%
5	2.845	465	468	470	rBV	263	150	0.01%	0.002%
6	2.916	488	490	495	rVB2	384	324	0.03%	0.004%
7	2.944	495	499	501	rBV2	339	322	0.03%	0.004%
8	3.115	548	552	553	rBV	206	158	0.02%	0.002%
9	3.189	567	575	580	rBV3	718	1189	0.12%	0.014%
10	3.227	584	587	589	rBV2	256	166	0.02%	0.002%
11	3.366	627	630	633	rVB	464	218	0.02%	0.003%
12	3.436	649	652	656	rBV	253	201	0.02%	0.002%
13	3.472	661	663	665	rVB	318	154	0.02%	0.002%
14	3.491	666	669	670	rBV2	366	244	0.02%	0.003%
15	3.526	676	680	682	rBV2	318	183	0.02%	0.002%
16	3.559	688	690	697	rVB2	342	407	0.04%	0.005%
17	3.661	720	722	725	rBV	189	144	0.01%	0.002%
18	3.800	762	765	768	rVB	216	129	0.01%	0.002%
19	3.896	792	795	798	rBV2	288	226	0.02%	0.003%
20	4.022	831	834	839	rVB	295	155	0.02%	0.002%
21	4.047	839	842	847	rBV2	254	239	0.02%	0.003%
22	4.102	856	859	862	rBV2	202	135	0.01%	0.002%
23	4.195	885	888	892	rBV	348	278	0.03%	0.003%
24	4.276	910	913	915	rBV	235	156	0.02%	0.002%
25	4.362	938	940	946	rVV2	230	264	0.03%	0.003%
26	4.459	967	970	973	rBV	236	140	0.01%	0.002%
27	4.520	985	989	994	rBV2	351	427	0.04%	0.005%
28	4.549	994	998	1001	rVB2	293	259	0.03%	0.003%
29	4.620	1007	1020	1045	rBV	112531	266283	26.03%	3.240%
30	5.063	1142	1158	1181	rBV	198602	435896	42.60%	5.304%
31	5.179	1192	1194	1198	rBV	374	297	0.03%	0.004%
32	5.375	1253	1255	1259	rBV	420	293	0.03%	0.004%
33	5.427	1265	1271	1274	rBV2	210	232	0.02%	0.003%
34	5.443	1274	1276	1279	rVB2	264	164	0.02%	0.002%
35	5.462	1280	1282	1284	rBV	302	183	0.02%	0.002%
36	5.514	1290	1298	1303	rBV2	345	566	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048499.D
 Acq On : 10 May 2022 18:21
 Operator : SY/MD
 Sample : N2736-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.575	1314	1317	1319	rBV2	308	178	0.02%	0.002%
38	5.620	1329	1331	1333	rBV	224	136	0.01%	0.002%
39	5.726	1342	1364	1382	rBV2	370572	1023112	100.00%	12.450%
40	5.951	1430	1434	1435	rBV2	268	206	0.02%	0.003%
41	6.041	1458	1462	1466	rBV3	780	783	0.08%	0.010%
42	6.108	1479	1483	1487	rBV2	413	426	0.04%	0.005%
43	6.150	1490	1496	1499	rBV	380	505	0.05%	0.006%
44	6.250	1513	1527	1554	rBV	339148	639246	62.48%	7.779%
45	6.530	1606	1614	1622	rVB6	1377	2533	0.25%	0.031%
46	6.690	1647	1664	1687	rBV	234819	457839	44.75%	5.571%
47	6.880	1720	1723	1724	rBV2	356	225	0.02%	0.003%
48	6.890	1724	1726	1730	rVB2	338	211	0.02%	0.003%
49	6.909	1730	1732	1734	rBV	280	127	0.01%	0.002%
50	7.031	1767	1770	1771	rBV	247	149	0.01%	0.002%
51	7.060	1775	1779	1783	rVB2	467	431	0.04%	0.005%
52	7.185	1811	1818	1830	rVB4	1842	3303	0.32%	0.040%
53	7.449	1897	1900	1903	rBV2	232	130	0.01%	0.002%
54	7.478	1903	1909	1914	rVB2	242	320	0.03%	0.004%
55	7.504	1915	1917	1920	rBV2	210	154	0.02%	0.002%
56	7.565	1923	1936	1952	rBV	129685	227369	22.22%	2.767%
57	7.687	1967	1974	1981	rBV3	1330	1901	0.19%	0.023%
58	7.729	1985	1987	1990	rVB2	309	147	0.01%	0.002%
59	7.771	1996	2000	2005	rBV	212	232	0.02%	0.003%
60	7.793	2005	2007	2009	rBV2	413	189	0.02%	0.002%
61	7.899	2026	2040	2055	rBV	451260	779281	76.17%	9.483%
62	8.179	2114	2127	2147	rBV	96509	162089	15.84%	1.972%
63	8.439	2205	2208	2210	rBV2	367	283	0.03%	0.003%
64	8.472	2210	2218	2227	rVV3	2715	4739	0.46%	0.058%
65	8.510	2227	2230	2235	rVB	350	252	0.02%	0.003%
66	8.565	2241	2247	2250	rBV3	570	532	0.05%	0.006%
67	8.581	2250	2252	2255	rVB2	368	178	0.02%	0.002%
68	8.632	2255	2268	2301	rBV	342187	621820	60.78%	7.567%
69	8.906	2349	2353	2359	rBV2	295	470	0.05%	0.006%
70	8.947	2363	2366	2368	rBV	273	140	0.01%	0.002%
71	9.018	2385	2388	2389	rBV	309	161	0.02%	0.002%
72	9.253	2459	2461	2463	rBV	187	129	0.01%	0.002%
73	9.327	2478	2484	2486	rBV	385	419	0.04%	0.005%
74	9.417	2498	2512	2536	rBV	484646	798743	78.07%	9.719%
75	9.976	2684	2686	2689	rVB2	264	137	0.01%	0.002%
76	10.047	2705	2708	2710	rBV2	207	151	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048499.D
 Acq On : 10 May 2022 18:21
 Operator : SY/MD
 Sample : N2736-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.356	2802	2804	2807	rVB	496	239	0.02%	0.003%
78	10.378	2807	2811	2815	rBV2	221	230	0.02%	0.003%
79	10.562	2865	2868	2870	rBV	236	155	0.02%	0.002%
80	10.642	2890	2893	2896	rBV	245	196	0.02%	0.002%
81	10.758	2916	2929	2950	rBV	361371	577991	56.49%	7.033%
82	10.899	2964	2973	2980	rBV4	2587	3969	0.39%	0.048%
83	11.153	3048	3052	3055	rVB	260	208	0.02%	0.003%
84	11.176	3055	3059	3064	rBV2	326	381	0.04%	0.005%
85	11.253	3081	3083	3086	rVB	322	184	0.02%	0.002%
86	11.333	3104	3108	3112	rBV2	324	342	0.03%	0.004%
87	11.410	3130	3132	3136	rBV2	246	129	0.01%	0.002%
88	11.603	3190	3192	3195	rBV	241	164	0.02%	0.002%
89	11.619	3195	3197	3201	rVV	275	164	0.02%	0.002%
90	11.700	3219	3222	3228	rBV3	554	483	0.05%	0.006%
91	11.812	3244	3257	3277	rBV	520776	829364	81.06%	10.092%
92	11.960	3299	3303	3305	rBV3	394	369	0.04%	0.004%
93	12.028	3320	3324	3327	rBV2	373	270	0.03%	0.003%
94	12.192	3362	3375	3392	rBV	472891	778216	76.06%	9.470%
95	12.973	3615	3618	3620	rBV2	422	290	0.03%	0.004%
96	13.185	3682	3684	3687	rBV	324	223	0.02%	0.003%
97	13.233	3697	3699	3704	rVB4	562	417	0.04%	0.005%
98	13.577	3804	3806	3807	rBV	369	162	0.02%	0.002%
99	14.777	4177	4179	4182	rBV	620	312	0.03%	0.004%
100	15.700	4464	4466	4472	rVB4	1148	786	0.08%	0.010%




Sum of corrected areas: 8218015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048499.D
Acq On : 10 May 2022 18:21
Operator : SY/MD
Sample : N2736-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

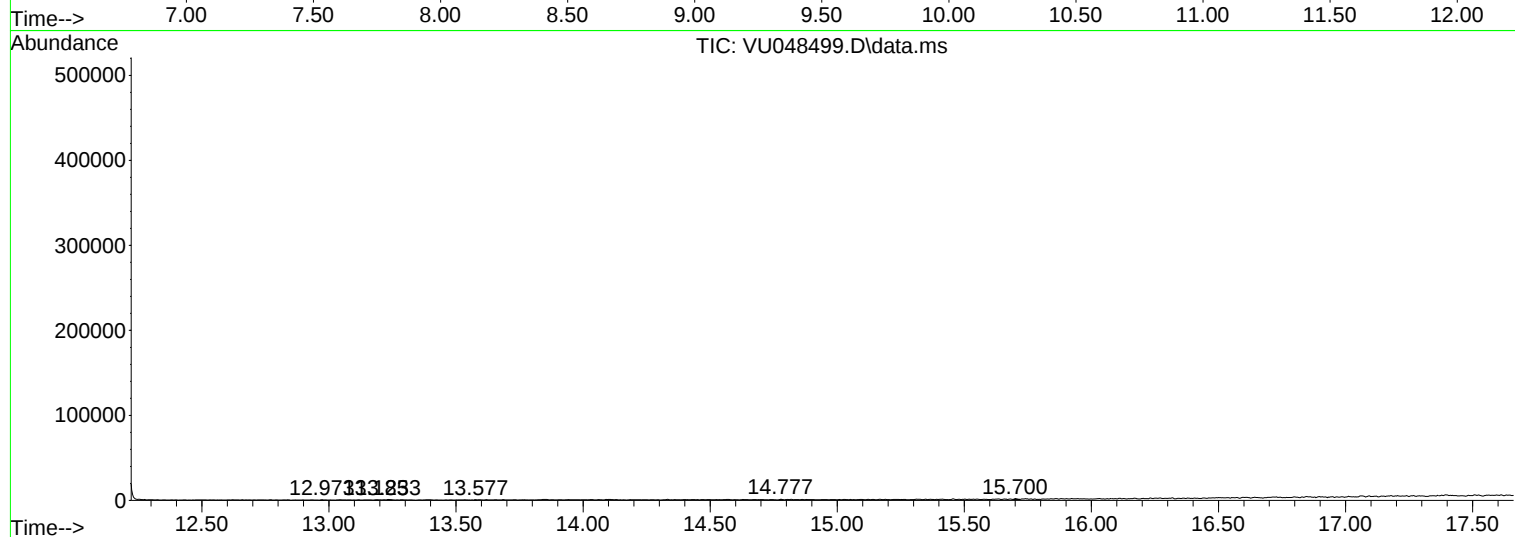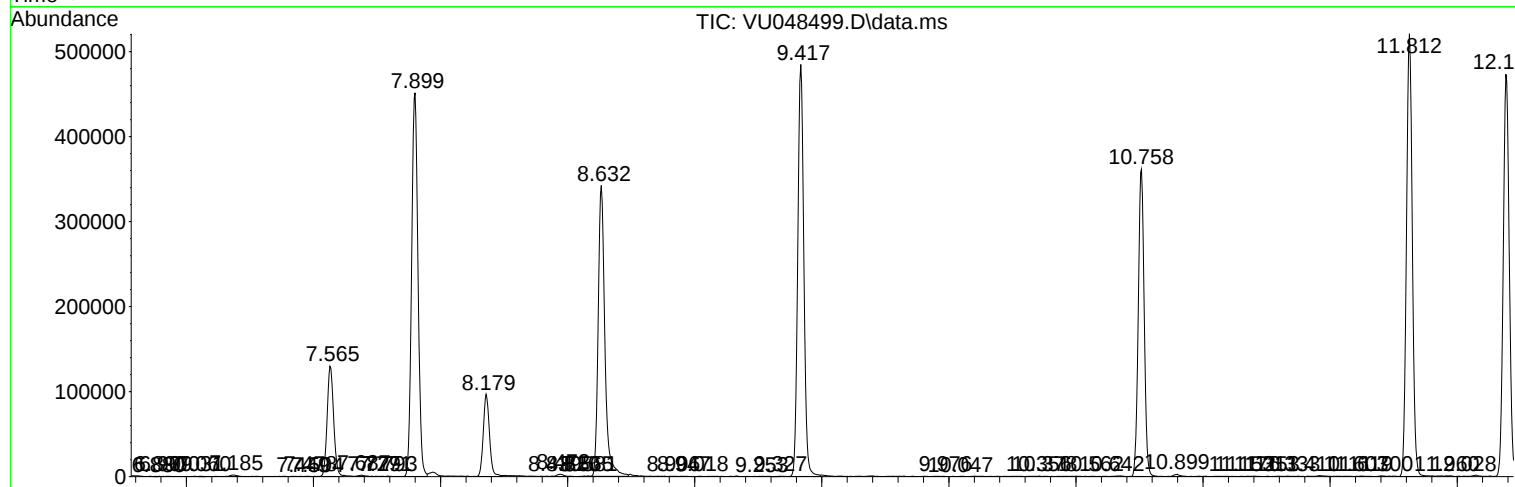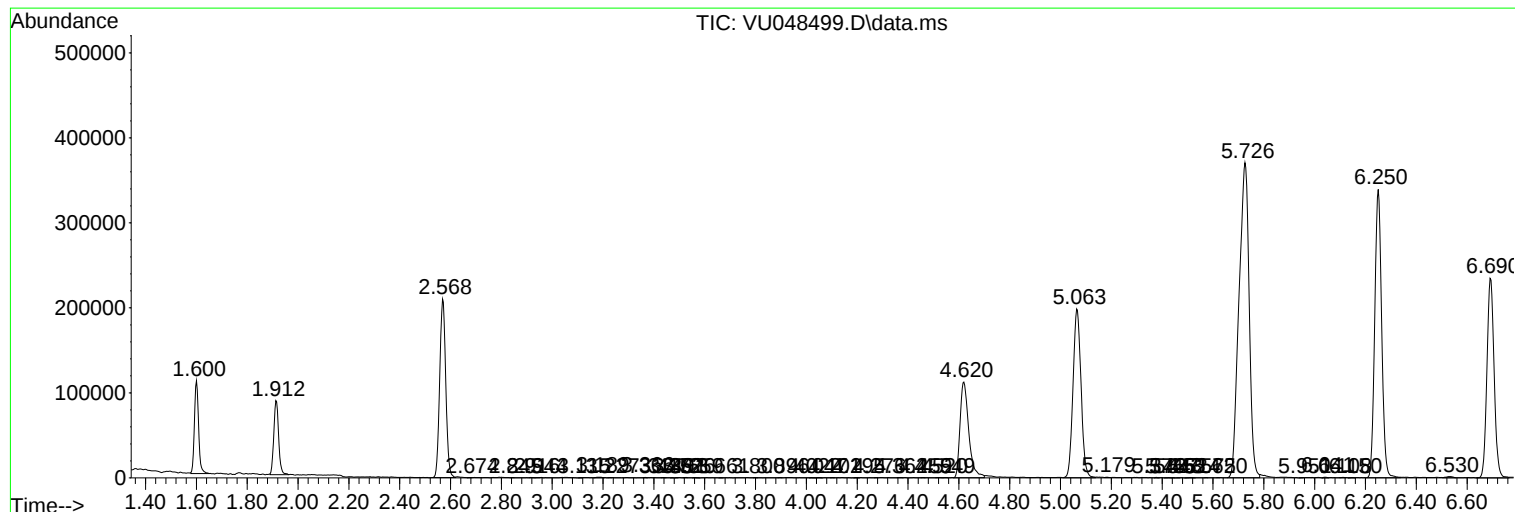

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048499.D
Acq On : 10 May 2022 18:21
Operator : SY/MD
Sample : N2736-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
Data File : VU048499.D
Acq On : 10 May 2022 18:21
Operator : SY/MD
Sample : N2736-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------