
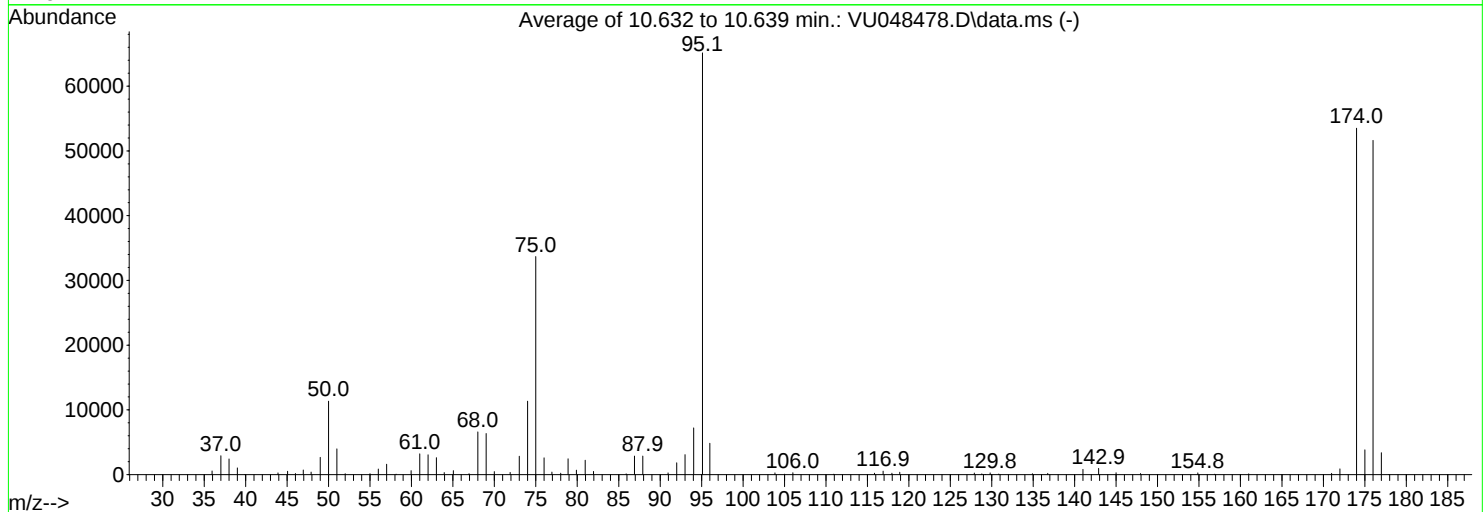


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051022\
 Data File : VU048478.D
 Acq On : 10 May 2022 09:00
 Operator : SY/MD
 Sample : BFB082
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB082

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis
 Last Update : Fri May 13 03:54:05 2022

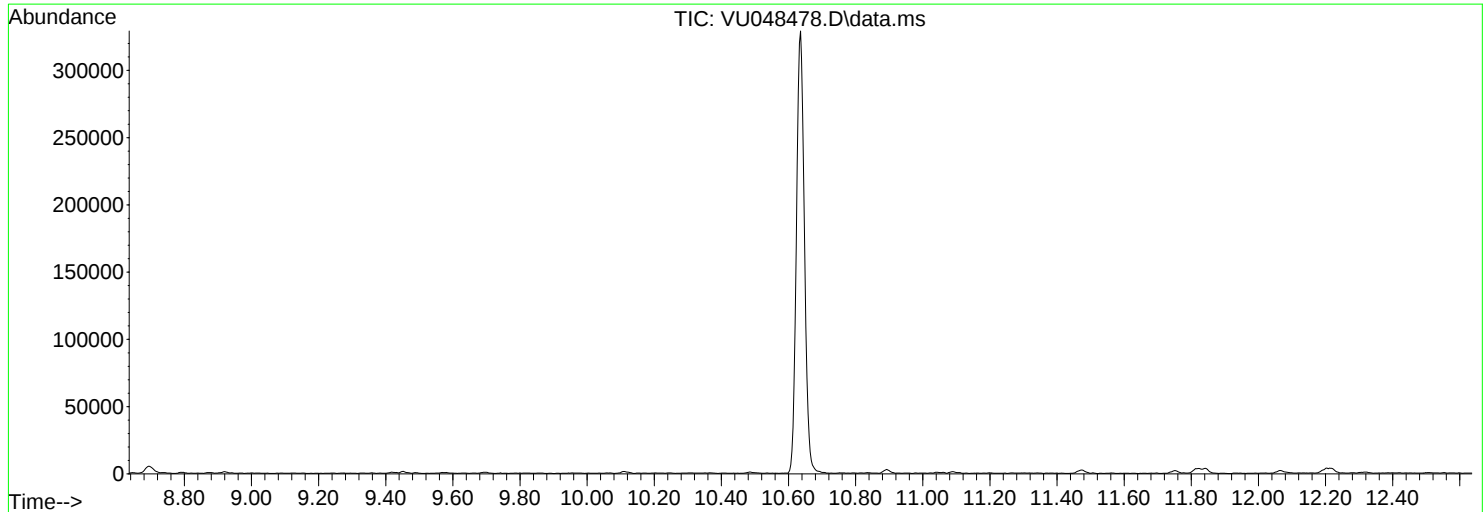

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	11338	PASS
75	95	30	80	51.7	33699	PASS
95	95	100	100	100.0	65149	PASS
96	95	5	9	7.4	4849	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.1	53499	PASS
175	174	5	9	7.1	3820	PASS
176	174	95	101	96.5	51624	PASS
177	176	5	9	6.6	3399	PASS

m/z	Abundance
36.00	581.0
37.00	2888.0
38.00	2395.0
39.00	1030.0
39.90	216.0
44.00	623.0
45.00	541.0
46.10	174.0
47.00	670.0
47.90	347.0
49.00	2470.0
50.00	10805.0
51.00	3727.0
52.00	166.0
55.00	137.0
56.00	798.0
57.00	1415.0
59.90	649.0
61.00	3154.0
62.00	3058.0
63.00	2582.0
63.90	290.0
65.00	655.0
67.00	135.0
68.00	5913.0
69.00	6013.0
70.00	456.0
71.90	295.0
73.00	2813.0
74.00	10897.0
75.00	32208.0
76.00	2580.0
77.00	363.0
78.00	180.0
78.90	2248.0
79.90	657.0
81.00	2128.0
81.90	497.0
85.90	108.0
86.90	2670.0
87.90	2742.0
90.90	231.0
92.00	1745.0
93.00	3316.0
94.00	6911.0
95.10	62656.0
96.00	4374.0
103.90	300.0
106.00	307.0
110.90	100.0
115.80	202.0
116.90	495.0
118.00	233.0
118.90	411.0
127.90	224.0
128.70	105.0
129.80	256.0
130.90	148.0
134.90	201.0
136.80	212.0
141.00	865.0
142.90	882.0
145.00	293.0
148.00	177.0
154.90	244.0
156.90	123.0
161.10	130.0
171.10	136.0
172.00	937.0
174.00	52448.0
175.00	3767.0
176.00	51000.0
177.00	3228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
39.90	202.0
43.90	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	551.0
37.00	2905.0
38.00	2397.0
39.00	983.0
39.90	233.0
43.90	662.0
45.10	485.0
45.90	151.0
46.90	763.0
47.90	423.0
49.00	2820.0
50.00	11531.0
51.00	4060.0
52.00	136.0
55.00	155.0
56.00	901.0
57.00	1715.0
58.10	122.0
60.00	580.0
61.00	3140.0
62.00	3007.0
63.00	2632.0
64.00	330.0
65.10	562.0
66.90	176.0
68.00	7066.0
69.00	6586.0
70.00	513.0
71.90	385.0
73.00	2808.0
74.00	11472.0
75.00	33944.0
76.00	2533.0
76.90	405.0
78.00	259.0
78.90	2552.0
79.90	725.0
80.90	2267.0
81.90	498.0
85.90	142.0
86.90	3011.0
87.90	2886.0
91.00	292.0
92.00	1890.0
93.00	2785.0
94.10	7282.0
95.10	65792.0
96.00	5217.0
103.80	271.0
105.00	133.0
106.00	256.0
115.90	239.0
116.90	582.0
117.90	212.0
118.90	338.0
127.90	245.0
128.90	153.0
129.80	291.0
134.90	113.0
136.80	179.0
141.00	772.0
142.90	1044.0
145.00	293.0
147.90	153.0
154.80	260.0
160.90	124.0
171.00	225.0
172.00	797.0
174.00	53048.0
175.00	3752.0
176.00	50536.0
177.00	3493.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	606.0
37.00	2953.0
38.00	2468.0
39.00	1096.0
39.90	225.0
43.90	662.0
45.00	551.0
46.00	168.0
47.00	724.0
47.90	440.0
49.00	2705.0
50.00	11677.0
51.00	4116.0
52.00	183.0
55.00	159.0
56.00	891.0
57.00	1660.0
58.20	107.0
60.00	608.0
61.00	3335.0
62.00	3103.0
63.00	2643.0
63.90	326.0
65.10	611.0
66.90	145.0
68.00	6784.0
69.00	6458.0
70.00	462.0
71.90	335.0
73.00	2922.0
74.00	11676.0
75.00	34944.0
76.00	2692.0
76.90	425.0
78.00	231.0
78.90	2578.0
79.90	726.0
81.00	2294.0
82.00	509.0
85.90	126.0
86.90	2925.0
87.90	3005.0
91.00	294.0
92.00	1866.0
93.00	3188.0
94.00	7472.0
95.10	67000.0
96.00	4956.0
103.80	264.0
105.00	124.0
106.00	310.0
111.00	101.0
115.90	242.0
116.90	542.0
118.00	205.0
118.90	369.0
127.90	241.0
128.80	122.0
129.20	104.0
129.80	311.0
130.80	123.0
134.90	154.0
136.70	204.0
141.00	839.0
142.90	950.0
145.00	310.0
148.00	196.0
154.90	290.0
156.90	103.0
161.00	145.0
171.00	203.0
172.00	908.0
174.00	55000.0
175.00	3942.0
176.00	53336.0
177.00	3476.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082