

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054137.D
 Acq On : 10 May 2023 11:15
 Operator : JC/MD
 Sample : VU0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK096

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	71200	84663	11.16%	1.470%
2	1.906	169	176	190	rVB	60042	82427	10.86%	1.432%
3	2.562	368	380	398	rBV	137796	226741	29.88%	3.938%
4	2.681	415	417	421	rBV2	372	232	0.03%	0.004%
5	2.845	463	468	471	rBV2	406	322	0.04%	0.006%
6	3.038	523	528	529	rBV3	1862	1553	0.20%	0.027%
7	3.244	589	592	595	rVB2	255	142	0.02%	0.002%
8	3.359	616	628	636	rVB6	2079	3378	0.45%	0.059%
9	3.491	668	669	670	rBV6	157	46	0.01%	0.001%
10	3.530	679	681	683	rBV	150	81	0.01%	0.001%
11	3.784	758	760	761	rBV2	153	75	0.01%	0.001%
12	4.141	868	871	872	rBV	152	101	0.01%	0.002%
13	4.182	881	884	887	rBV	172	96	0.01%	0.002%
14	4.327	926	929	931	rBV3	315	206	0.03%	0.004%
15	4.414	954	956	958	rBV	280	151	0.02%	0.003%
16	4.430	958	961	964	rVB	361	283	0.04%	0.005%
17	4.446	964	966	967	rBV	183	97	0.01%	0.002%
18	4.459	967	970	974	rVB2	238	226	0.03%	0.004%
19	4.507	983	985	986	rBV	244	120	0.02%	0.002%
20	4.549	996	998	999	rBV	180	96	0.01%	0.002%
21	4.620	1008	1020	1045	rBV	61733	158489	20.89%	2.753%
22	4.935	1116	1118	1121	rBV	142	110	0.01%	0.002%
23	4.954	1121	1124	1126	rBV3	256	174	0.02%	0.003%
24	5.057	1140	1156	1175	rBV	139838	309218	40.76%	5.370%
25	5.253	1216	1217	1218	rBV	211	68	0.01%	0.001%
26	5.298	1225	1231	1233	rBV2	867	785	0.10%	0.014%
27	5.353	1246	1248	1250	rBV	167	99	0.01%	0.002%
28	5.366	1250	1252	1253	rBV	452	211	0.03%	0.004%
29	5.414	1266	1267	1268	rVB	110	21	0.00%	0.000%
30	5.430	1270	1272	1273	rBV	122	33	0.00%	0.001%
31	5.494	1289	1292	1293	rBV	315	200	0.03%	0.003%
32	5.552	1307	1310	1311	rBV	145	67	0.01%	0.001%
33	5.565	1311	1314	1321	rVB2	155	164	0.02%	0.003%
34	5.597	1321	1324	1325	rBV2	129	56	0.01%	0.001%
35	5.719	1341	1362	1395	rBV2	272279	758716	100.00%	13.177%
36	5.960	1434	1437	1440	rVB2	166	111	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054137.D
 Acq On : 10 May 2023 11:15
 Operator : JC/MD
 Sample : VU0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK096

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.989	1443	1446	1451	rVB	365	326	0.04%	0.006%
38	6.012	1451	1453	1456	rBB	159	101	0.01%	0.002%
39	6.031	1456	1459	1462	rBV2	267	197	0.03%	0.003%
40	6.047	1462	1464	1467	rVB2	254	138	0.02%	0.002%
41	6.182	1504	1506	1508	rBV	166	69	0.01%	0.001%
42	6.243	1512	1525	1545	rBV	249199	470424	62.00%	8.170%
43	6.494	1602	1603	1605	rBV	122	65	0.01%	0.001%
44	6.530	1605	1614	1624	rVV6	3428	6473	0.85%	0.112%
45	6.600	1634	1636	1640	rVB	240	105	0.01%	0.002%
46	6.684	1648	1662	1679	rBV	177203	347571	45.81%	6.037%
47	6.841	1707	1711	1712	rBV	221	168	0.02%	0.003%
48	6.964	1747	1749	1753	rVB	190	97	0.01%	0.002%
49	7.073	1781	1783	1785	rBV	139	97	0.01%	0.002%
50	7.102	1786	1792	1799	rVB3	593	933	0.12%	0.016%
51	7.186	1813	1818	1820	rBV2	878	846	0.11%	0.015%
52	7.269	1840	1844	1845	rBV2	243	146	0.02%	0.003%
53	7.375	1873	1877	1878	rBV2	248	176	0.02%	0.003%
54	7.433	1892	1895	1899	rBV	199	130	0.02%	0.002%
55	7.520	1920	1922	1923	rBV	153	62	0.01%	0.001%
56	7.562	1923	1935	1955	rBV	88794	160639	21.17%	2.790%
57	7.784	1998	2004	2005	rBV4	1033	801	0.11%	0.014%
58	7.893	2021	2038	2073	rBV	331252	583942	76.96%	10.142%
59	8.041	2082	2084	2089	rBV2	207	124	0.02%	0.002%
60	8.063	2089	2091	2098	rVB3	449	420	0.06%	0.007%
61	8.092	2098	2100	2103	rBV	252	136	0.02%	0.002%
62	8.176	2115	2126	2143	rBV	64842	110223	14.53%	1.914%
63	8.298	2162	2164	2165	rBV	150	61	0.01%	0.001%
64	8.391	2190	2193	2195	rBV2	867	647	0.09%	0.011%
65	8.439	2205	2208	2211	rBV2	245	188	0.02%	0.003%
66	8.465	2213	2216	2221	rVB3	339	268	0.04%	0.005%
67	8.507	2226	2229	2233	rVV2	210	192	0.03%	0.003%
68	8.552	2236	2243	2249	rVB3	1482	2282	0.30%	0.040%
69	8.629	2255	2267	2303	rBV2	179655	349570	46.07%	6.071%
70	8.851	2335	2336	2338	rBV2	225	85	0.01%	0.001%
71	8.909	2351	2354	2355	rBV	346	185	0.02%	0.003%
72	9.060	2396	2401	2408	rBV2	236	335	0.04%	0.006%
73	9.089	2408	2410	2413	rVV2	326	157	0.02%	0.003%
74	9.295	2468	2474	2476	rBV	275	314	0.04%	0.005%
75	9.366	2495	2496	2497	rBV	125	32	0.00%	0.001%
76	9.411	2498	2510	2536	rVV	333039	561975	74.07%	9.760%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054137.D
 Acq On : 10 May 2023 11:15
 Operator : JC/MD
 Sample : VU0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK096

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	9.684	2591	2595	2596	rBV2	1051	743	0.10%	0.013%
78	9.829	2638	2640	2641	rBV2	128	28	0.00%	0.000%
79	10.050	2707	2709	2710	rBV2	187	61	0.01%	0.001%
80	10.208	2755	2758	2759	rBV	211	109	0.01%	0.002%
81	10.404	2818	2819	2820	rBV	118	29	0.00%	0.001%
82	10.481	2838	2843	2853	rVB4	2258	2767	0.36%	0.048%
83	10.636	2887	2891	2900	rVB4	903	966	0.13%	0.017%
84	10.751	2915	2927	2943	rBV	242770	396175	52.22%	6.881%
85	10.906	2972	2975	2979	rBV	297	180	0.02%	0.003%
86	10.996	2999	3003	3005	rBV2	270	224	0.03%	0.004%
87	11.086	3024	3031	3035	rBV2	1384	1692	0.22%	0.029%
88	11.410	3129	3132	3134	rBV	223	117	0.02%	0.002%
89	11.468	3143	3150	3158	rVB2	1855	2649	0.35%	0.046%
90	11.745	3230	3236	3243	rVB4	2838	4029	0.53%	0.070%
91	11.806	3243	3255	3276	rBV	334728	536088	70.66%	9.311%
92	12.189	3361	3374	3393	rBV	330751	549031	72.36%	9.535%
93	12.311	3411	3412	3413	rBV	220	75	0.01%	0.001%
94	12.944	3606	3609	3614	rBV2	311	277	0.04%	0.005%
95	13.221	3689	3695	3706	rVB3	2714	4243	0.56%	0.074%
96	13.841	3880	3888	3896	rBV5	4761	7008	0.92%	0.122%
97	14.086	3954	3964	3979	rBV	7270	13579	1.79%	0.236%
98	14.330	4033	4040	4050	rVB3	4949	7442	0.98%	0.129%




Sum of corrected areas: 5757770

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054137.D
Acq On : 10 May 2023 11:15
Operator : JC/MD
Sample : VU0510MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

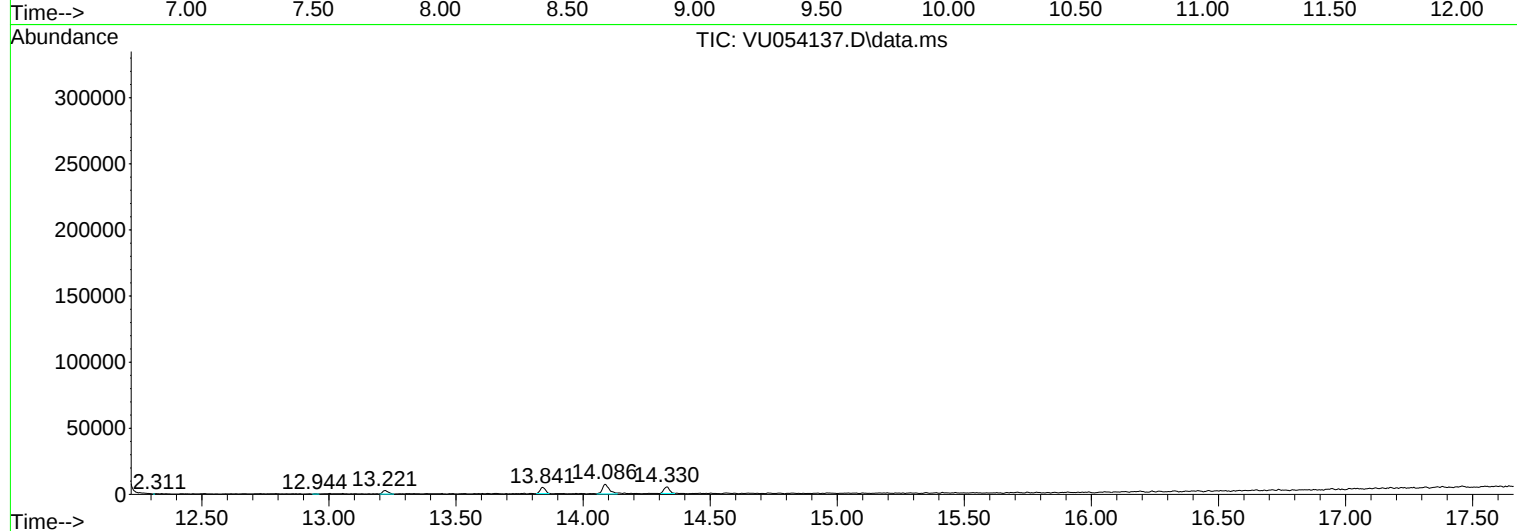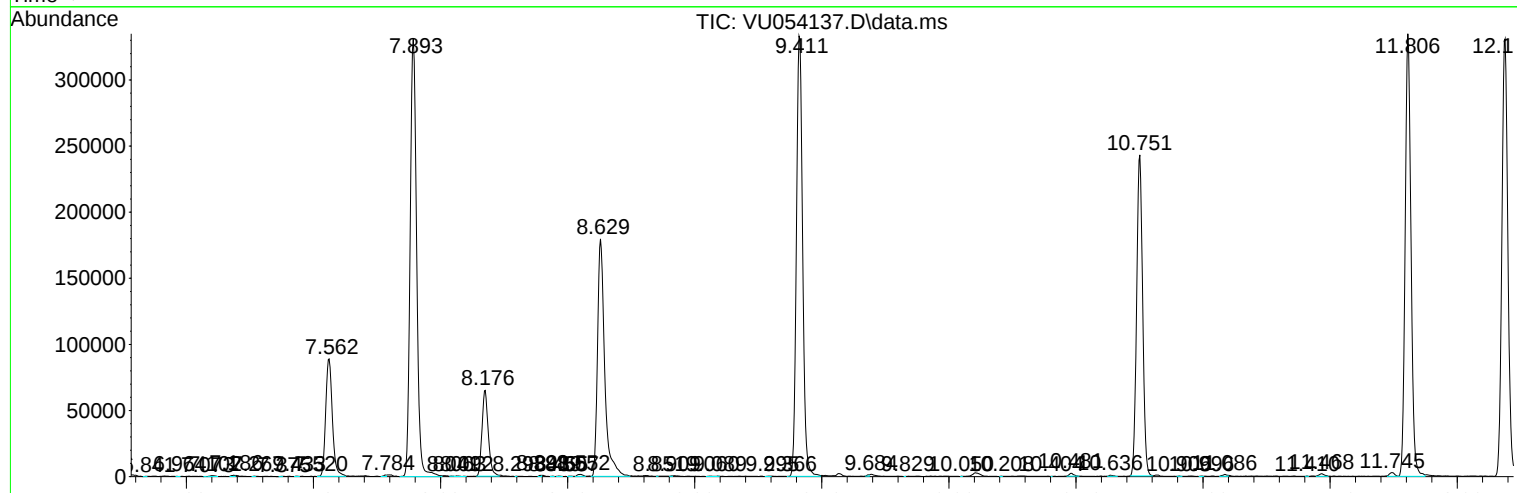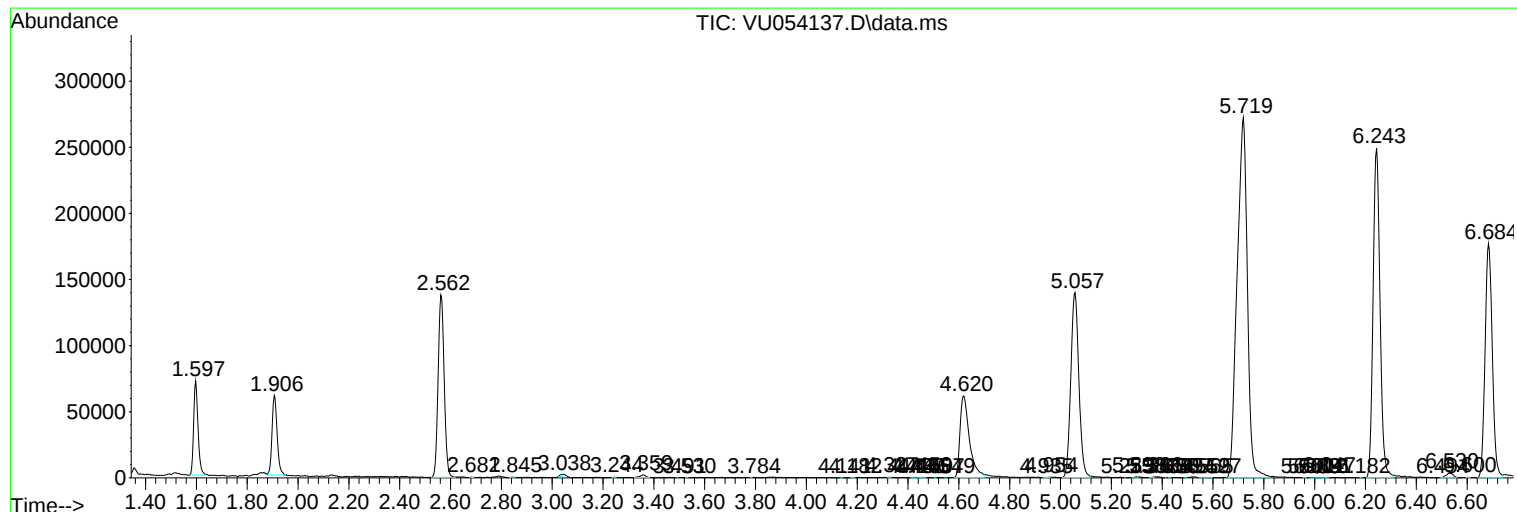

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054137.D
Acq On : 10 May 2023 11:15
Operator : JC/MD
Sample : VU0510MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054137.D
Acq On : 10 May 2023 11:15
Operator : JC/MD
Sample : VU0510MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc