

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054140.D
 Acq On : 10 May 2023 13:16
 Operator : JC/MD
 Sample : 02694-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	97	rVB	66671	80934	10.78%	1.363%
2	1.909	170	177	193	rVB	56439	80280	10.69%	1.352%
3	2.562	369	380	394	rBV	133274	217387	28.96%	3.661%
4	2.706	422	425	429	rVB4	393	299	0.04%	0.005%
5	3.038	523	528	529	rBV3	1050	852	0.11%	0.014%
6	3.179	560	572	585	rBV2	4167	9402	1.25%	0.158%
7	3.353	624	626	628	rBV2	207	83	0.01%	0.001%
8	3.391	636	638	646	rBV	145	127	0.02%	0.002%
9	3.452	653	657	661	rVB2	374	352	0.05%	0.006%
10	3.478	661	665	674	rBV2	281	342	0.05%	0.006%
11	3.620	707	709	712	rBV2	214	115	0.02%	0.002%
12	3.636	712	714	718	rVB	205	100	0.01%	0.002%
13	3.748	746	749	751	rVB	154	81	0.01%	0.001%
14	3.777	755	758	765	rBV2	210	230	0.03%	0.004%
15	3.816	769	770	771	rBV2	133	39	0.01%	0.001%
16	3.870	784	787	789	rBV	235	106	0.01%	0.002%
17	4.102	856	859	861	rBV	174	99	0.01%	0.002%
18	4.160	876	877	878	rBV	136	39	0.01%	0.001%
19	4.208	887	892	896	rBV2	406	503	0.07%	0.008%
20	4.231	896	899	903	rVB2	250	225	0.03%	0.004%
21	4.356	934	938	942	rVB2	228	163	0.02%	0.003%
22	4.375	942	944	947	rBV	156	87	0.01%	0.001%
23	4.481	974	977	979	rBV2	236	160	0.02%	0.003%
24	4.497	979	982	984	rVV	193	146	0.02%	0.002%
25	4.620	1008	1020	1054	rBV	60792	164882	21.96%	2.777%
26	4.922	1111	1114	1115	rBV	241	95	0.01%	0.002%
27	4.957	1122	1125	1129	rVB2	215	192	0.03%	0.003%
28	5.057	1139	1156	1179	rBV	139509	309581	41.24%	5.214%
29	5.276	1221	1224	1227	rBV	353	157	0.02%	0.003%
30	5.314	1232	1236	1238	rBV2	378	270	0.04%	0.005%
31	5.337	1240	1243	1247	rVV2	306	220	0.03%	0.004%
32	5.459	1278	1281	1284	rBV	166	110	0.01%	0.002%
33	5.591	1321	1322	1323	rBV	100	25	0.00%	0.000%
34	5.603	1323	1326	1330	rVB	232	150	0.02%	0.003%
35	5.626	1330	1333	1335	rBV	247	139	0.02%	0.002%
36	5.719	1339	1362	1386	rBV2	270010	750677	100.00%	12.644%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054140.D
 Acq On : 10 May 2023 13:16
 Operator : JC/MD
 Sample : 02694-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.919	1421	1424	1426	rBV2	201	152	0.02%	0.003%
38	5.967	1437	1439	1440	rBV	115	42	0.01%	0.001%
39	6.163	1498	1500	1501	rBV	114	44	0.01%	0.001%
40	6.192	1507	1509	1512	rBV2	202	119	0.02%	0.002%
41	6.243	1512	1525	1542	rBV	272931	515368	68.65%	8.680%
42	6.526	1606	1613	1620	rBV4	2412	4006	0.53%	0.067%
43	6.623	1641	1643	1644	rVB4	237	72	0.01%	0.001%
44	6.684	1649	1662	1683	rBV	179492	350845	46.74%	5.909%
45	6.890	1724	1726	1728	rBV	158	105	0.01%	0.002%
46	6.947	1742	1744	1750	rVB	170	81	0.01%	0.001%
47	6.976	1750	1753	1756	rBV	206	138	0.02%	0.002%
48	7.066	1778	1781	1784	rBV	224	170	0.02%	0.003%
49	7.189	1811	1819	1821	rBV2	687	782	0.10%	0.013%
50	7.221	1826	1829	1831	rVB2	282	188	0.03%	0.003%
51	7.253	1832	1839	1841	rBV	249	320	0.04%	0.005%
52	7.288	1849	1850	1851	rBV	128	31	0.00%	0.001%
53	7.298	1851	1853	1855	rVB	164	69	0.01%	0.001%
54	7.356	1869	1871	1874	rBV	196	94	0.01%	0.002%
55	7.433	1893	1895	1897	rBV	129	43	0.01%	0.001%
56	7.484	1908	1911	1914	rBV	198	113	0.02%	0.002%
57	7.562	1923	1935	1954	rBV	92604	164060	21.85%	2.763%
58	7.677	1969	1971	1974	rBV2	331	212	0.03%	0.004%
59	7.735	1987	1989	1990	rBV2	286	99	0.01%	0.002%
60	7.758	1994	1996	1998	rVB	179	71	0.01%	0.001%
61	7.793	2003	2007	2009	rBV2	472	339	0.05%	0.006%
62	7.893	2024	2038	2057	rBV	336770	585734	78.03%	9.865%
63	8.095	2098	2101	2106	rVB2	315	193	0.03%	0.003%
64	8.176	2114	2126	2149	rBV	65889	112657	15.01%	1.897%
65	8.404	2192	2197	2202	rBV2	222	238	0.03%	0.004%
66	8.468	2208	2217	2225	rBV2	1238	1956	0.26%	0.033%
67	8.542	2237	2240	2243	rBV2	259	191	0.03%	0.003%
68	8.571	2247	2249	2254	rVB	356	300	0.04%	0.005%
69	8.629	2255	2267	2295	rBV2	176488	352596	46.97%	5.939%
70	8.809	2314	2323	2325	rBV2	489	617	0.08%	0.010%
71	9.015	2384	2387	2389	rBV2	199	118	0.02%	0.002%
72	9.047	2396	2397	2398	rBV2	121	29	0.00%	0.000%
73	9.253	2459	2461	2462	rBV	133	32	0.00%	0.001%
74	9.414	2497	2511	2533	rBV	369296	623400	83.05%	10.500%
75	9.616	2572	2574	2575	rBV	147	60	0.01%	0.001%
76	9.648	2581	2584	2589	rBV	241	211	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054140.D
 Acq On : 10 May 2023 13:16
 Operator : JC/MD
 Sample : 02694-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	9.864	2647	2651	2653	rBV	247	196	0.03%	0.003%
78	9.996	2689	2692	2695	rVB	178	77	0.01%	0.001%
79	10.098	2722	2724	2728	rVB2	529	350	0.05%	0.006%
80	10.471	2838	2840	2842	rBV	292	173	0.02%	0.003%
81	10.613	2882	2884	2886	rVB	145	57	0.01%	0.001%
82	10.632	2887	2890	2892	rBV	296	206	0.03%	0.003%
83	10.751	2915	2927	2947	rVB	251592	406088	54.10%	6.840%
84	10.970	2993	2995	2999	rVB	273	143	0.02%	0.002%
85	11.066	3022	3025	3027	rBV	265	140	0.02%	0.002%
86	11.459	3144	3147	3148	rBV	320	207	0.03%	0.003%
87	11.526	3164	3168	3170	rBV	356	288	0.04%	0.005%
88	11.806	3243	3255	3279	rBV	389228	613949	81.79%	10.341%
89	12.188	3361	3374	3394	rBV	353726	579895	77.25%	9.767%
90	13.102	3656	3658	3660	rBV	294	136	0.02%	0.002%
91	13.227	3692	3697	3700	rBV3	543	487	0.06%	0.008%
92	13.471	3771	3773	3775	rBV2	287	148	0.02%	0.002%
93	13.600	3811	3813	3816	rBV2	268	117	0.02%	0.002%




Sum of corrected areas: 5937201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054140.D
Acq On : 10 May 2023 13:16
Operator : JC/MD
Sample : 02694-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

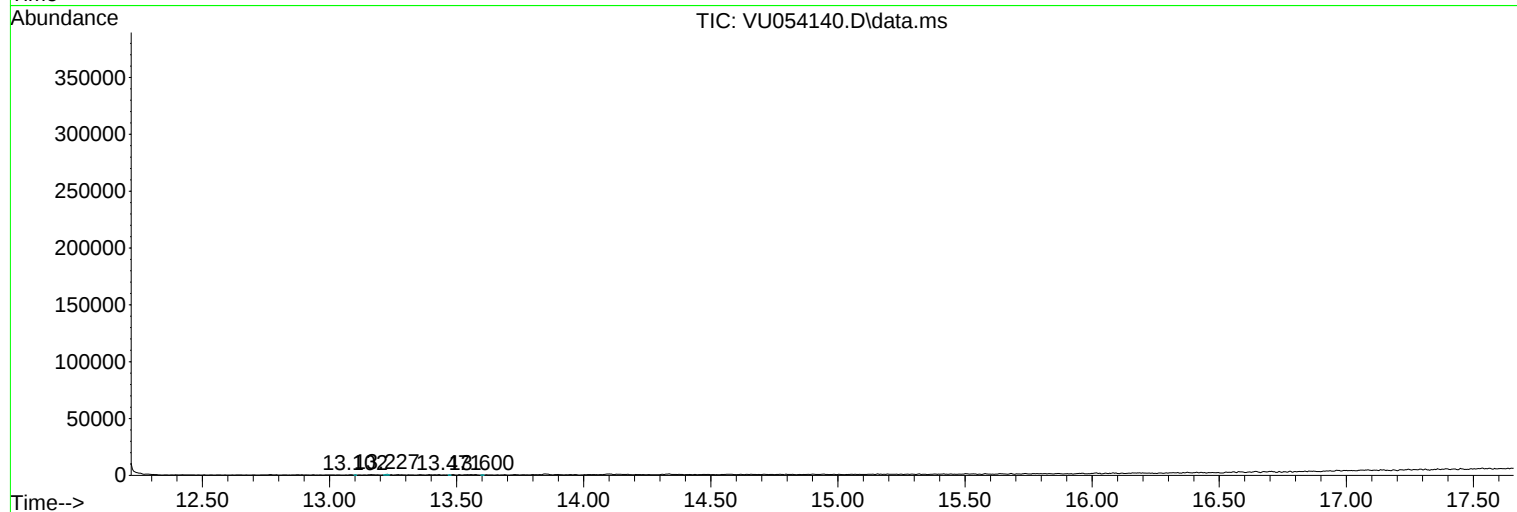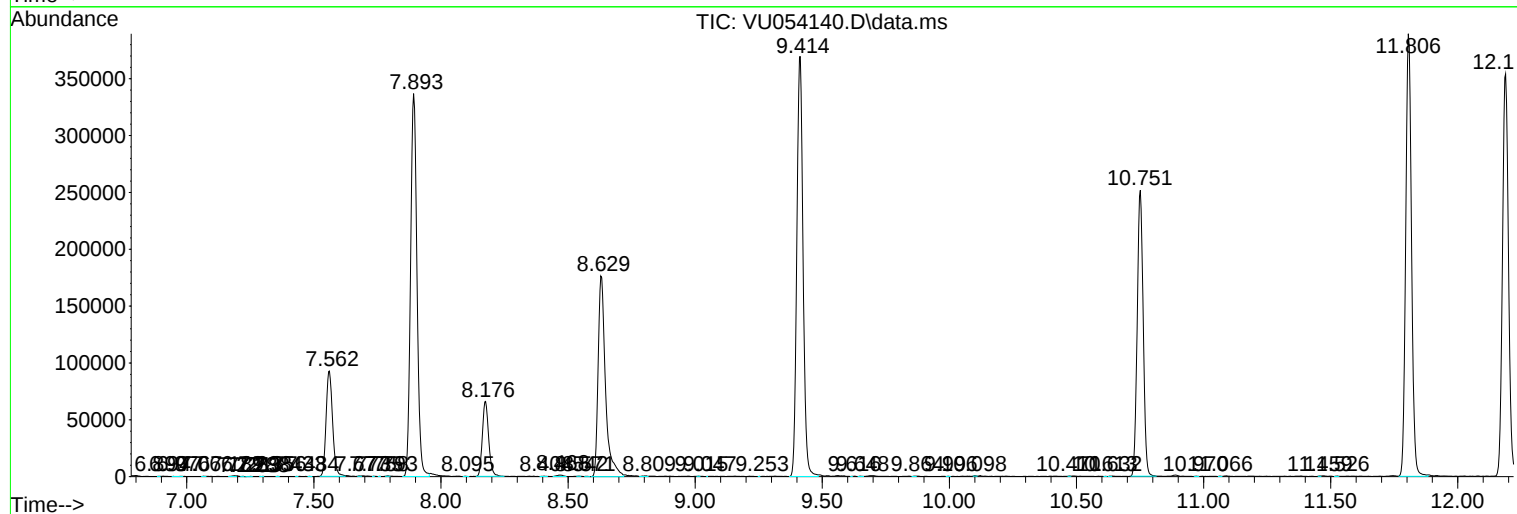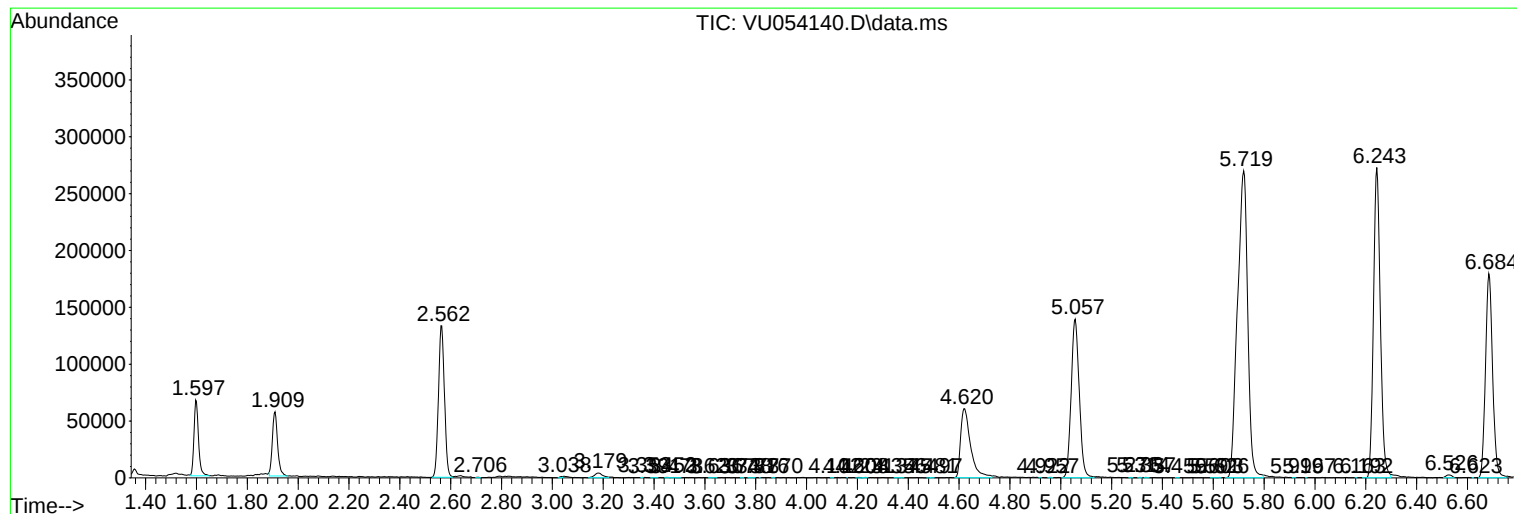

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054140.D
Acq On : 10 May 2023 13:16
Operator : JC/MD
Sample : 02694-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054140.D
Acq On : 10 May 2023 13:16
Operator : JC/MD
Sample : 02694-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------