

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054145.D
 Acq On : 10 May 2023 15:14
 Operator : JC/MD
 Sample : 02694-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	90950	110401	13.49%	1.679%
2	1.906	169	176	193	rVB	72394	101543	12.41%	1.544%
3	2.562	368	380	395	rBV	159763	262386	32.06%	3.990%
4	3.182	559	573	585	rBV2	2346	5586	0.68%	0.085%
5	3.256	595	596	597	rBV	219	68	0.01%	0.001%
6	3.372	630	632	633	rBV	150	46	0.01%	0.001%
7	3.469	660	662	664	rBV	163	91	0.01%	0.001%
8	3.478	664	665	669	rVB	257	98	0.01%	0.001%
9	3.501	669	672	673	rBV2	199	113	0.01%	0.002%
10	3.536	680	683	685	rBV2	196	117	0.01%	0.002%
11	3.549	685	687	689	rVV	134	56	0.01%	0.001%
12	3.588	696	699	701	rBV	158	68	0.01%	0.001%
13	3.658	718	721	723	rBV2	177	121	0.01%	0.002%
14	3.764	750	754	757	rBV2	189	151	0.02%	0.002%
15	3.880	789	790	791	rBV2	99	27	0.00%	0.000%
16	3.890	791	793	796	rVB	151	48	0.01%	0.001%
17	3.912	797	800	802	rBV	224	118	0.01%	0.002%
18	3.983	820	822	824	rBV	193	121	0.01%	0.002%
19	4.031	834	837	840	rVB	157	65	0.01%	0.001%
20	4.086	852	854	858	rVB	237	97	0.01%	0.001%
21	4.144	869	872	876	rBV2	191	188	0.02%	0.003%
22	4.170	876	880	883	rBV2	285	203	0.02%	0.003%
23	4.227	894	898	907	rVB2	234	252	0.03%	0.004%
24	4.279	909	914	919	rBV2	314	440	0.05%	0.007%
25	4.314	922	925	926	rBV	264	185	0.02%	0.003%
26	4.353	935	937	938	rBV	136	37	0.00%	0.001%
27	4.366	939	941	945	rVB2	199	140	0.02%	0.002%
28	4.417	952	957	960	rBV2	371	368	0.04%	0.006%
29	4.510	984	986	990	rVB2	183	125	0.02%	0.002%
30	4.536	992	994	997	rBV	138	120	0.01%	0.002%
31	4.617	1008	1019	1043	rBV2	63295	158182	19.33%	2.406%
32	4.977	1128	1131	1132	rBV	126	71	0.01%	0.001%
33	5.057	1140	1156	1186	rBV	150939	335061	40.94%	5.096%
34	5.372	1250	1254	1256	rBV2	141	129	0.02%	0.002%
35	5.388	1257	1259	1260	rBV2	167	73	0.01%	0.001%
36	5.456	1277	1280	1283	rBV	258	250	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054145.D
 Acq On : 10 May 2023 15:14
 Operator : JC/MD
 Sample : 02694-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.552	1308	1310	1311	rBB	114	43	0.01%	0.001%
38	5.719	1341	1362	1388	rBV2	299640	818356	100.00%	12.445%
39	5.977	1436	1442	1444	rBV2	376	439	0.05%	0.007%
40	6.038	1458	1461	1464	rVB	414	274	0.03%	0.004%
41	6.112	1479	1484	1488	rBV2	349	448	0.05%	0.007%
42	6.243	1512	1525	1553	rBV	305624	585117	71.50%	8.898%
43	6.472	1594	1596	1599	rBV2	260	146	0.02%	0.002%
44	6.530	1605	1614	1623	rBV3	2231	3776	0.46%	0.057%
45	6.684	1648	1662	1694	rBV	191032	373468	45.64%	5.680%
46	6.800	1695	1698	1703	rVB3	810	674	0.08%	0.010%
47	6.896	1726	1728	1737	rVB2	471	578	0.07%	0.009%
48	6.932	1737	1739	1741	rBV	267	156	0.02%	0.002%
49	7.002	1758	1761	1765	rBV	207	200	0.02%	0.003%
50	7.041	1770	1773	1775	rBV	198	104	0.01%	0.002%
51	7.115	1794	1796	1797	rBV	143	48	0.01%	0.001%
52	7.166	1807	1812	1813	rBV	176	169	0.02%	0.003%
53	7.247	1835	1837	1838	rBV	132	35	0.00%	0.001%
54	7.353	1867	1870	1872	rBV	102	63	0.01%	0.001%
55	7.423	1891	1892	1895	rVB	294	121	0.01%	0.002%
56	7.443	1896	1898	1900	rBV	189	137	0.02%	0.002%
57	7.475	1905	1908	1913	rVB2	335	298	0.04%	0.005%
58	7.501	1913	1916	1918	rBV	213	161	0.02%	0.002%
59	7.559	1922	1934	1960	rVV2	108624	189104	23.11%	2.876%
60	7.751	1991	1994	1998	rBV2	225	205	0.03%	0.003%
61	7.768	1998	1999	2003	rVV	118	75	0.01%	0.001%
62	7.893	2025	2038	2055	rBV	377256	647357	79.10%	9.845%
63	8.173	2114	2125	2146	rBV	77813	132548	16.20%	2.016%
64	8.301	2159	2165	2167	rBV2	362	266	0.03%	0.004%
65	8.324	2167	2172	2174	rVB	231	193	0.02%	0.003%
66	8.504	2225	2228	2230	rBV	112	66	0.01%	0.001%
67	8.562	2243	2246	2250	rBV	214	134	0.02%	0.002%
68	8.629	2256	2267	2302	rBV2	184703	352396	43.06%	5.359%
69	8.832	2327	2330	2332	rVB2	238	112	0.01%	0.002%
70	8.883	2344	2346	2347	rBV2	210	73	0.01%	0.001%
71	9.002	2382	2383	2384	rBV2	109	26	0.00%	0.000%
72	9.095	2408	2412	2418	rVB	322	256	0.03%	0.004%
73	9.121	2418	2420	2423	rBV	146	61	0.01%	0.001%
74	9.163	2430	2433	2436	rBV	279	174	0.02%	0.003%
75	9.353	2489	2492	2493	rBV	228	137	0.02%	0.002%
76	9.411	2497	2510	2536	rBV	419733	707263	86.42%	10.756%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054145.D
 Acq On : 10 May 2023 15:14
 Operator : JC/MD
 Sample : 02694-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JREP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

77	9.626	2574	2577	2579	rBV2	166	118	0.01%	0.002%
78	9.758	2615	2618	2619	rBV2	202	97	0.01%	0.001%
79	9.796	2627	2630	2631	rBV	189	102	0.01%	0.002%
80	10.427	2824	2826	2829	rBV2	219	138	0.02%	0.002%
81	10.751	2915	2927	2945	rBV	261949	421372	51.49%	6.408%
82	11.166	3053	3056	3058	rBV	246	167	0.02%	0.003%
83	11.552	3174	3176	3179	rBV	259	137	0.02%	0.002%
84	11.655	3205	3208	3209	rBV	188	79	0.01%	0.001%
85	11.754	3236	3239	3241	rBV	347	149	0.02%	0.002%
86	11.806	3243	3255	3274	rBV	449044	706397	86.32%	10.743%
87	12.005	3314	3317	3318	rBV	219	127	0.02%	0.002%
88	12.076	3337	3339	3341	rVB	296	120	0.01%	0.002%
89	12.124	3351	3354	3357	rBV	239	174	0.02%	0.003%
90	12.189	3361	3374	3401	rVV	399818	653899	79.90%	9.944%
91	12.475	3460	3463	3464	rBV	253	122	0.01%	0.002%


Sum of corrected areas: 6575600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054145.D
Acq On : 10 May 2023 15:14
Operator : JC/MD
Sample : 02694-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

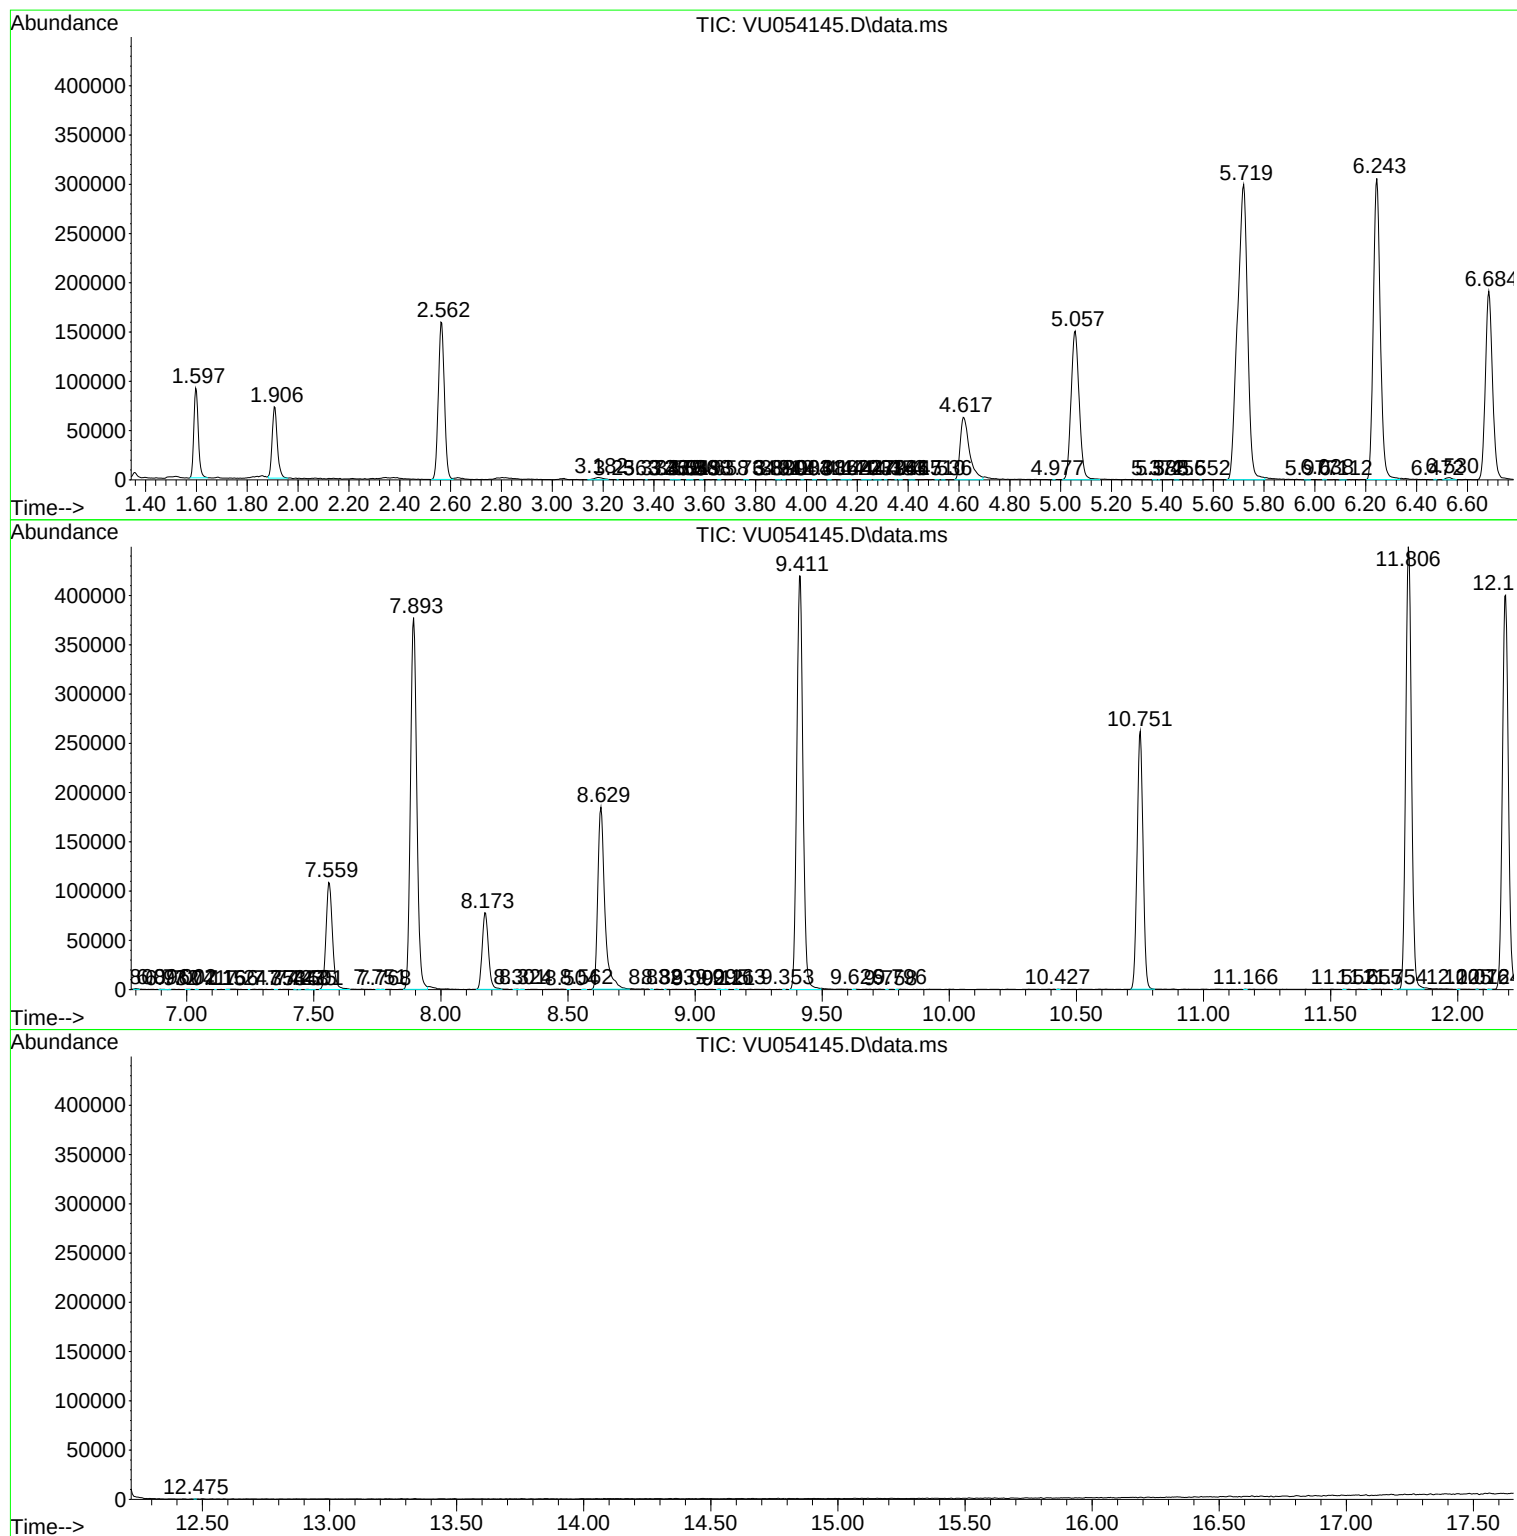

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054145.D
Acq On : 10 May 2023 15:14
Operator : JC/MD
Sample : 02694-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054145.D
Acq On : 10 May 2023 15:14
Operator : JC/MD
Sample : 02694-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JREP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------