

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054147.D
 Acq On : 10 May 2023 16:00
 Operator : JC/MD
 Sample : 02694-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rVB	100968	123791	13.71%	1.746%
2	1.906	168	176	192	rVB	79642	112280	12.43%	1.583%
3	2.562	366	380	398	rBV	180635	295907	32.77%	4.172%
4	2.703	422	424	427	rBV	409	206	0.02%	0.003%
5	2.851	468	470	471	rBV	173	93	0.01%	0.001%
6	2.932	493	495	498	rVB	212	77	0.01%	0.001%
7	3.041	520	529	544	rBV3	5792	10981	1.22%	0.155%
8	3.179	563	572	577	rBV2	1150	1936	0.21%	0.027%
9	3.629	710	712	715	rBV2	148	98	0.01%	0.001%
10	3.790	760	762	763	rBV2	147	43	0.00%	0.001%
11	3.832	772	775	778	rVB	253	150	0.02%	0.002%
12	3.886	790	792	794	rVB	149	63	0.01%	0.001%
13	3.922	800	803	809	rBV2	221	164	0.02%	0.002%
14	3.957	810	814	816	rVB2	149	113	0.01%	0.002%
15	3.983	819	822	824	rVB	236	133	0.01%	0.002%
16	4.060	843	846	848	rBV	220	122	0.01%	0.002%
17	4.112	861	862	863	rVB	220	42	0.00%	0.001%
18	4.150	870	874	879	rVB2	238	175	0.02%	0.002%
19	4.182	879	884	885	rBV	147	119	0.01%	0.002%
20	4.221	892	896	899	rBV	155	152	0.02%	0.002%
21	4.285	910	916	921	rBV2	384	536	0.06%	0.008%
22	4.375	941	944	947	rBB	177	115	0.01%	0.002%
23	4.401	950	952	956	rVB	181	87	0.01%	0.001%
24	4.449	962	967	971	rBV2	209	262	0.03%	0.004%
25	4.616	1008	1019	1052	rBV	65462	166032	18.39%	2.341%
26	4.948	1119	1122	1127	rVB2	278	198	0.02%	0.003%
27	4.989	1131	1135	1138	rBV	274	161	0.02%	0.002%
28	5.057	1140	1156	1181	rBV	166488	371704	41.16%	5.241%
29	5.250	1213	1216	1218	rBV	158	84	0.01%	0.001%
30	5.317	1234	1237	1245	rBB	209	197	0.02%	0.003%
31	5.404	1261	1264	1267	rBV2	242	220	0.02%	0.003%
32	5.468	1281	1284	1286	rBV	201	163	0.02%	0.002%
33	5.536	1302	1305	1310	rVB	253	162	0.02%	0.002%
34	5.555	1310	1311	1312	rBV	112	24	0.00%	0.000%
35	5.594	1320	1323	1325	rBV	213	138	0.02%	0.002%
36	5.719	1341	1362	1383	rBV2	331993	902999	100.00%	12.733%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054147.D
 Acq On : 10 May 2023 16:00
 Operator : JC/MD
 Sample : 02694-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	5.976	1438	1442	1444	rBV	277	164	0.02%	0.002%
38	6.092	1475	1478	1479	rBV	140	62	0.01%	0.001%
39	6.108	1480	1483	1487	rVB2	284	227	0.03%	0.003%
40	6.150	1492	1496	1497	rBV2	119	75	0.01%	0.001%
41	6.243	1511	1525	1552	rBV	310174	594975	65.89%	8.390%
42	6.468	1591	1595	1597	rBV2	187	137	0.02%	0.002%
43	6.481	1597	1599	1602	rVV	160	76	0.01%	0.001%
44	6.523	1604	1612	1624	rVB3	2880	5362	0.59%	0.076%
45	6.594	1630	1634	1635	rBV	358	301	0.03%	0.004%
46	6.684	1648	1662	1690	rBV	210634	411707	45.59%	5.805%
47	6.825	1705	1706	1710	rBV3	353	153	0.02%	0.002%
48	6.893	1726	1727	1729	rBV	251	91	0.01%	0.001%
49	6.954	1744	1746	1748	rVB	166	46	0.01%	0.001%
50	6.970	1748	1751	1752	rBV	188	88	0.01%	0.001%
51	7.018	1763	1766	1768	rVB	130	90	0.01%	0.001%
52	7.189	1817	1819	1823	rVB	477	303	0.03%	0.004%
53	7.240	1833	1835	1837	rBV	239	141	0.02%	0.002%
54	7.472	1905	1907	1912	rVB2	177	129	0.01%	0.002%
55	7.501	1915	1916	1921	rBB2	209	102	0.01%	0.001%
56	7.558	1922	1934	1954	rBV2	118639	210403	23.30%	2.967%
57	7.703	1976	1979	1983	rBV4	416	439	0.05%	0.006%
58	7.822	2013	2016	2018	rBV	213	132	0.01%	0.002%
59	7.835	2018	2020	2023	rVB	155	65	0.01%	0.001%
60	7.893	2024	2038	2057	rBV	419076	727126	80.52%	10.253%
61	8.173	2114	2125	2142	rBV	84601	144503	16.00%	2.038%
62	8.433	2202	2206	2211	rBV	297	341	0.04%	0.005%
63	8.472	2214	2218	2222	rBV2	443	403	0.04%	0.006%
64	8.629	2255	2267	2305	rBV2	198783	382584	42.37%	5.395%
65	8.787	2314	2316	2320	rBV	230	174	0.02%	0.002%
66	8.816	2324	2325	2329	rVB	309	155	0.02%	0.002%
67	8.951	2365	2367	2369	rBV	191	77	0.01%	0.001%
68	9.005	2383	2384	2388	rBV	142	77	0.01%	0.001%
69	9.118	2414	2419	2423	rBV	155	170	0.02%	0.002%
70	9.140	2423	2426	2430	rVV	189	132	0.01%	0.002%
71	9.163	2431	2433	2437	rVV	309	223	0.02%	0.003%
72	9.185	2438	2440	2444	rVB2	260	197	0.02%	0.003%
73	9.253	2457	2461	2467	rVB2	307	318	0.04%	0.004%
74	9.320	2480	2482	2484	rBV2	152	80	0.01%	0.001%
75	9.410	2498	2510	2532	rBV	421655	711232	78.76%	10.029%
76	9.671	2589	2591	2594	rVB	173	60	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
 Data File : VU054147.D
 Acq On : 10 May 2023 16:00
 Operator : JC/MD
 Sample : 02694-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	9.687	2594	2596	2597	rBV	195	67	0.01%	0.001%
78	9.748	2611	2615	2618	rBV2	233	200	0.02%	0.003%
79	9.809	2632	2634	2636	rBV	213	79	0.01%	0.001%
80	9.906	2661	2664	2668	rVB	278	222	0.02%	0.003%
81	10.076	2714	2717	2720	rVB	279	135	0.01%	0.002%
82	10.137	2729	2736	2740	rBV	402	430	0.05%	0.006%
83	10.269	2775	2777	2780	rVB	180	94	0.01%	0.001%
84	10.751	2914	2927	2948	rBV	282815	456436	50.55%	6.436%
85	10.970	2990	2995	2996	rBV2	269	232	0.03%	0.003%
86	11.134	3043	3046	3048	rBV	223	123	0.01%	0.002%
87	11.626	3196	3199	3200	rBV	213	103	0.01%	0.001%
88	11.668	3209	3212	3218	rVB2	240	231	0.03%	0.003%
89	11.806	3243	3255	3278	rBV	460649	723848	80.16%	10.207%
90	12.188	3361	3374	3397	rBV	442476	726265	80.43%	10.241%
91	12.417	3443	3445	3449	rBV	398	312	0.03%	0.004%
92	14.018	3941	3943	3946	rBV	373	225	0.02%	0.003%




Sum of corrected areas: 7091849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054147.D
Acq On : 10 May 2023 16:00
Operator : JC/MD
Sample : 02694-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

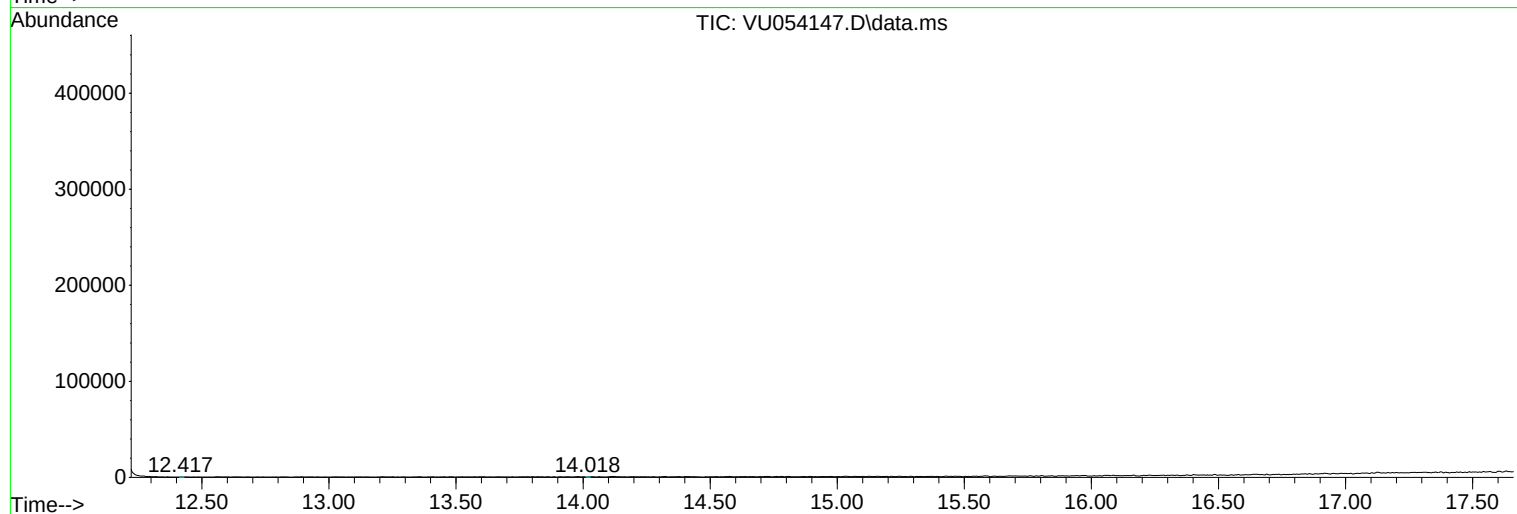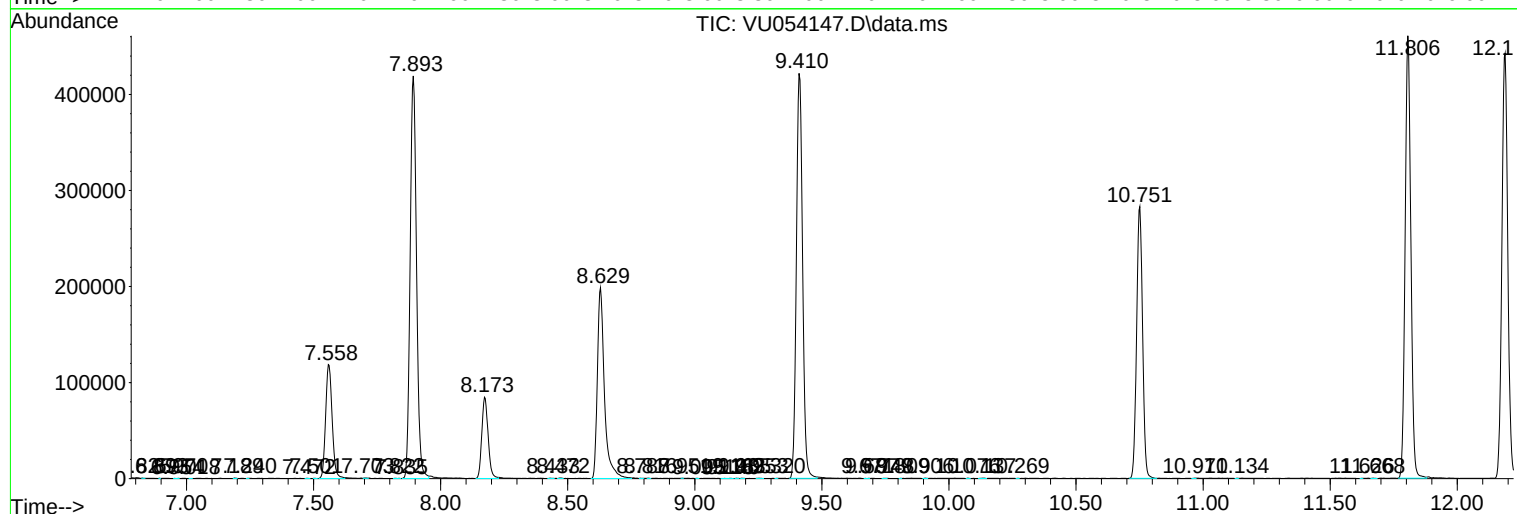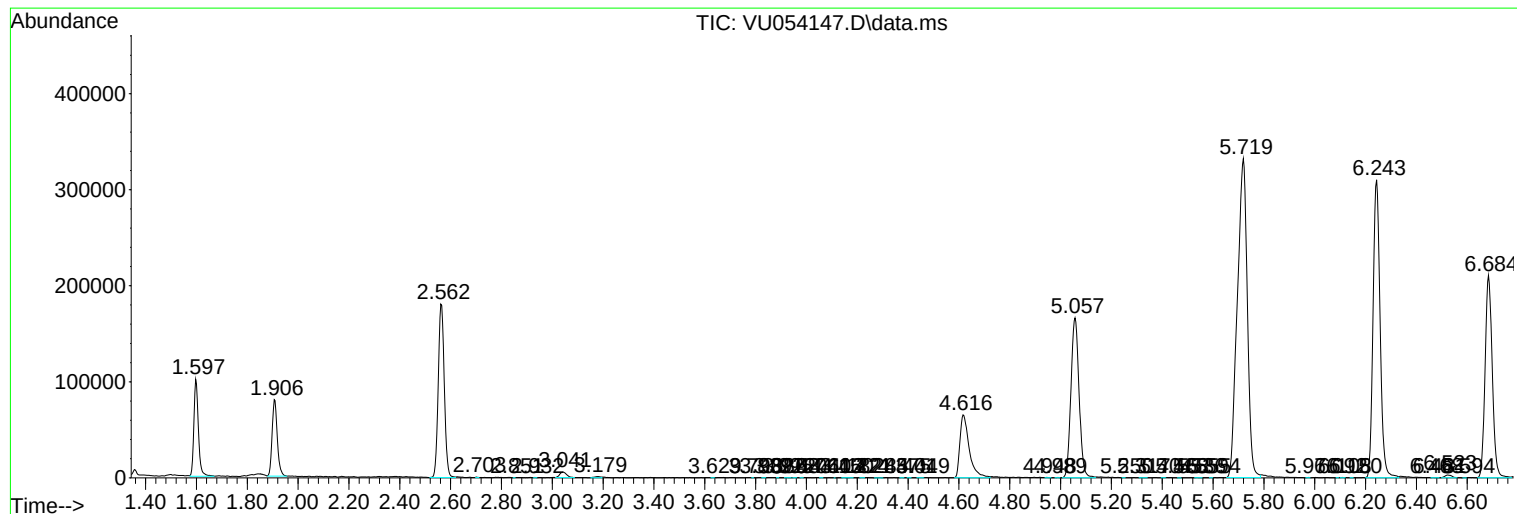

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054147.D
Acq On : 10 May 2023 16:00
Operator : JC/MD
Sample : 02694-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051023\
Data File : VU054147.D
Acq On : 10 May 2023 16:00
Operator : JC/MD
Sample : 02694-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------