


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU051118\
Data File : VU023791.D
Acq On : 11 May 2018 09:36
Operator : MD/SY
Sample : BFB49
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMUTR051018WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat May 12 02:07:11 2018

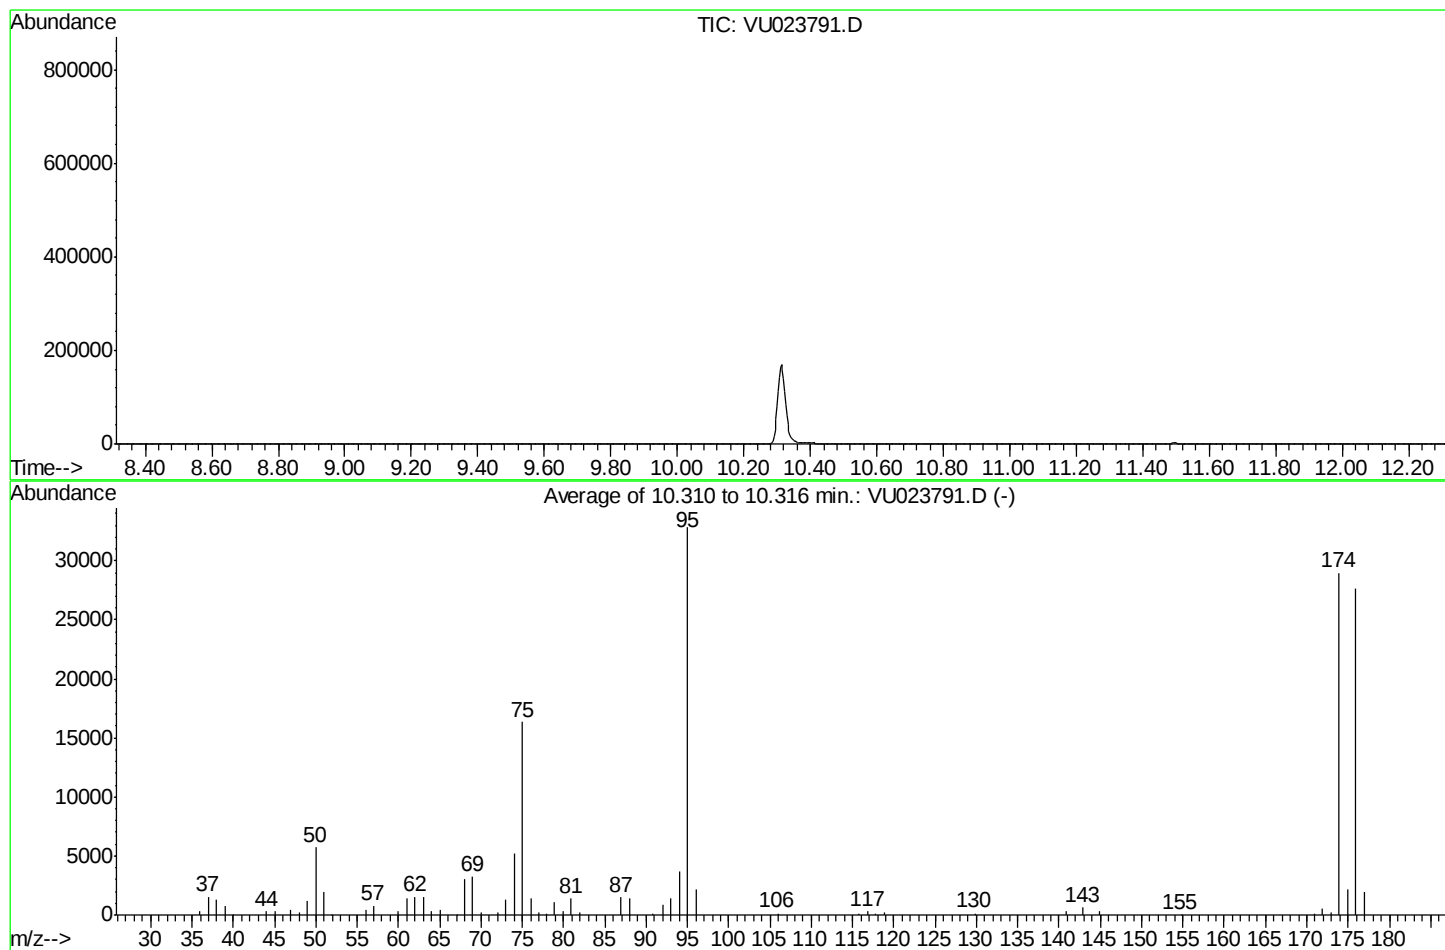

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	5741	PASS
75	95	30	80	49.8	16346	PASS
95	95	100	100	100.0	32834	PASS
96	95	5	9	6.7	2186	PASS
173	174	0.00	2	0.9	250	PASS
174	95	50	120	88.2	28960	PASS
175	174	5	9	7.3	2127	PASS
176	174	95	101	95.6	27680	PASS
177	176	5	9	7.2	1988	PASS

Scan 3011 (10.271 min): VU023791.D
BFB49

m/z	Abundance
39.90	165.0
44.00	330.0

m/z	Abundance
35.90	301.0
37.00	1591.0
37.90	1291.0
39.10	694.0
39.90	211.0
44.00	691.0
45.00	310.0
47.00	491.0
47.90	204.0
49.00	1191.0
50.00	5814.0
51.00	2081.0
51.90	124.0
56.10	429.0
57.00	773.0
60.00	366.0
61.00	1382.0
62.00	1573.0
63.00	1549.0
64.00	362.0
65.00	449.0
68.00	3065.0
69.00	3336.0
70.10	200.0
72.00	192.0
73.00	1318.0
74.00	5075.0
75.00	16512.0
76.00	1421.0
77.00	194.0
77.90	106.0
78.90	1160.0
80.00	259.0
80.90	1401.0
81.90	239.0
87.00	1443.0
88.00	1319.0
90.70	108.0
92.00	883.0
93.00	1338.0
94.00	3726.0
95.00	33176.0
96.00	2160.0
106.00	102.0
115.70	111.0
116.90	272.0
117.80	111.0
118.90	291.0
129.80	153.0
140.80	348.0
142.90	626.0
144.90	318.0
171.00	120.0
171.90	569.0
172.90	346.0
173.90	27984.0
174.90	2168.0
175.90	26960.0
176.90	1968.0

m/z	Abundance
35.90	331.0
37.00	1570.0
38.00	1348.0
39.00	765.0
39.90	196.0
44.00	676.0
45.00	336.0
46.90	423.0
48.00	222.0
49.00	1229.0
50.00	5927.0
51.00	2055.0
56.10	432.0
57.00	848.0
60.00	349.0
61.00	1378.0
62.00	1634.0
63.00	1513.0
64.00	376.0
65.00	482.0
68.00	3116.0
69.00	3303.0
70.10	189.0
72.00	200.0
73.00	1368.0
74.00	5308.0
75.00	16872.0
76.00	1483.0
77.10	220.0
78.00	121.0
78.90	1150.0
80.00	298.0
80.90	1419.0
81.90	227.0
87.00	1533.0
88.00	1412.0
90.80	102.0
92.00	834.0
93.00	1464.0
94.00	3858.0
95.00	33776.0
96.00	2274.0
105.90	132.0
115.70	116.0
116.90	298.0
117.80	110.0
118.90	252.0
129.80	141.0
140.80	357.0
142.90	672.0
144.90	321.0
154.80	102.0
170.90	111.0
171.90	605.0
173.00	405.0
173.90	29816.0
174.90	2198.0
175.90	28496.0
176.90	2027.0

m/z	Abundance
35.90	292.0
37.00	1440.0
38.00	1272.0
39.00	774.0
39.90	177.0
44.00	574.0
45.00	303.0
46.90	363.0
48.00	205.0
49.00	1130.0
50.00	5484.0
51.00	1864.0
56.00	418.0
56.90	811.0
60.00	285.0
61.00	1345.0
62.00	1491.0
63.00	1356.0
64.00	343.0
65.00	419.0
67.10	102.0
68.00	2926.0
69.00	3095.0
70.00	194.0
72.00	186.0
73.00	1327.0
74.00	5104.0
75.00	15654.0
76.00	1391.0
77.00	222.0
78.00	139.0
78.90	1075.0
80.00	291.0
80.90	1288.0
81.90	210.0
86.90	1469.0
88.00	1375.0
90.80	106.0
92.00	758.0
93.00	1439.0
94.00	3579.0
95.00	31552.0
96.00	2124.0
106.00	148.0
115.70	105.0
116.90	276.0
117.80	114.0
118.90	221.0
129.80	101.0
140.80	337.0
142.90	638.0
144.90	304.0
170.80	112.0
171.90	582.0
173.90	29080.0
174.90	2017.0
175.90	27584.0
176.90	1971.0