
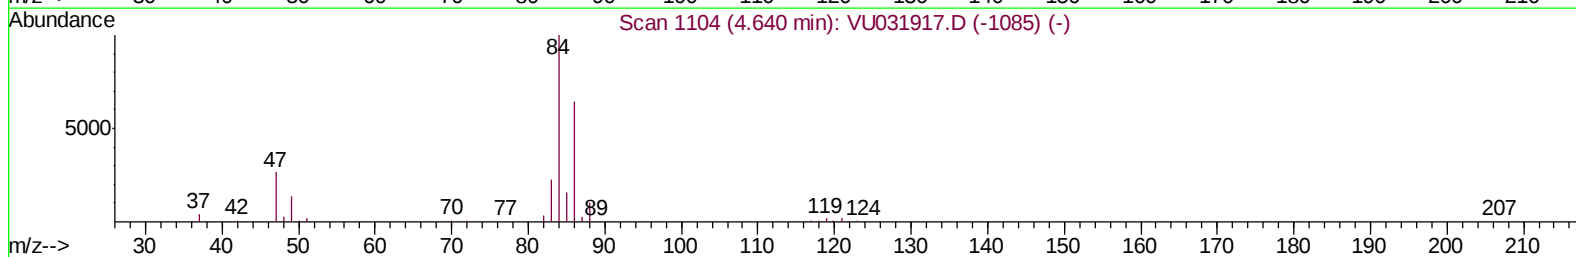
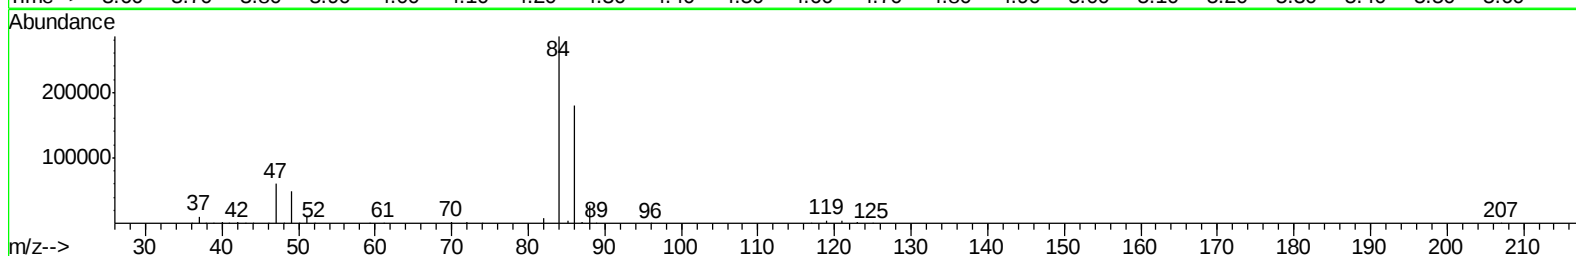


Data File : VU031920.D
Acq On : 11 May 2019 10:54
Operator : JC/SP
Sample : K2705-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 13 03:47:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 13 01:54:07 2019
Response via : Initial Calibration

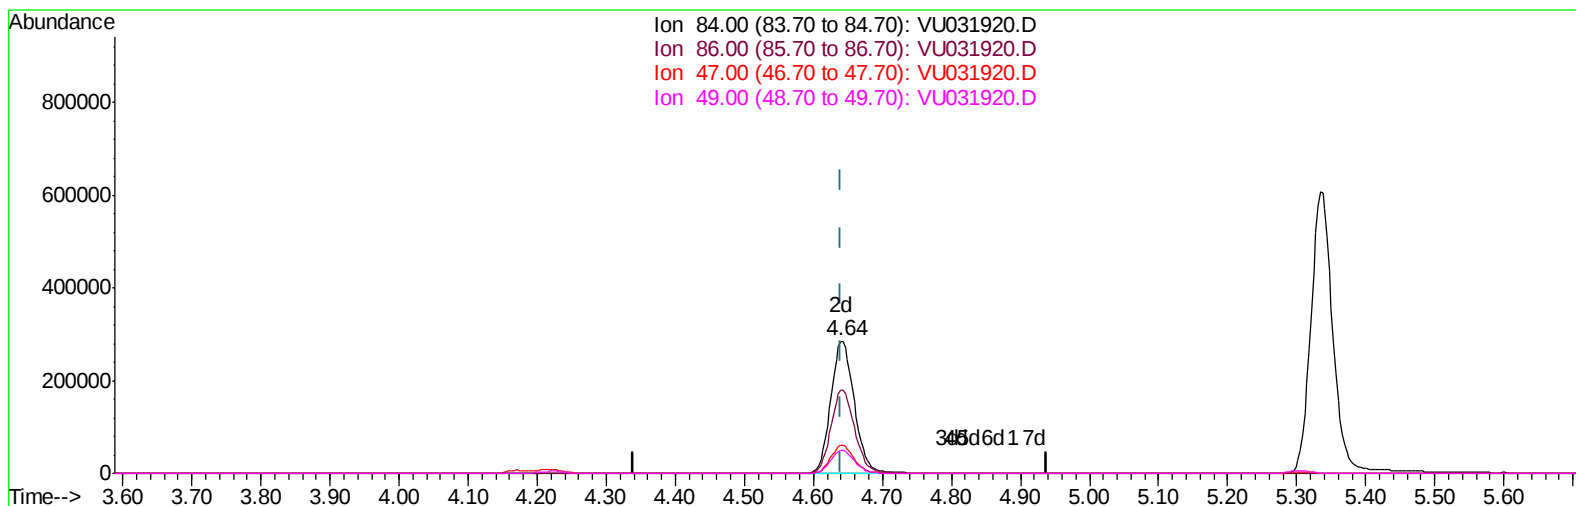

TIC: VU031920.D

(24) Chloroform-d (S)

4.640min (+0.000) 46.77ug/L m

response 666108

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	0.02#
47.00	45.70	0.01#
49.00	27.20	0.01#