
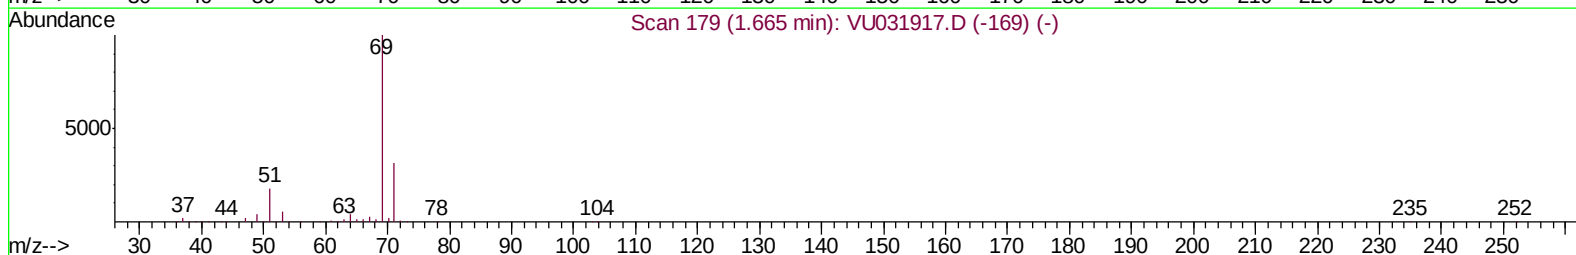
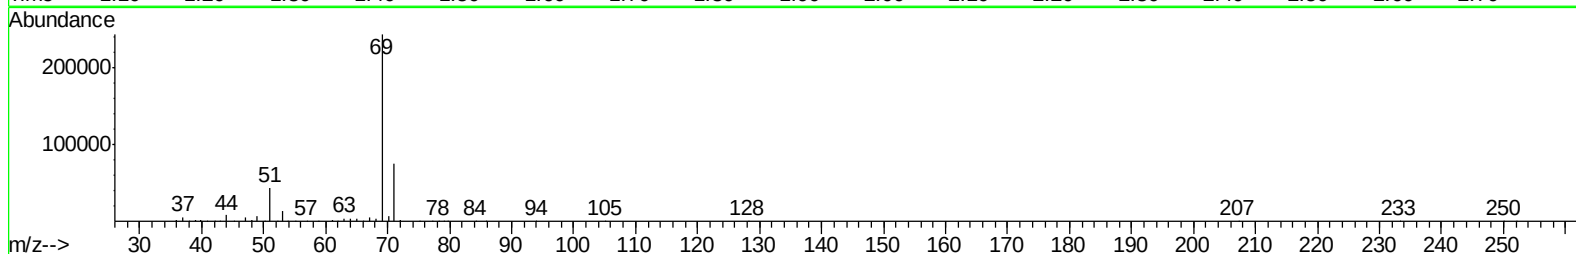


Data File : VU031922.D
Acq On : 11 May 2019 11:41
Operator : JC/SP
Sample : K2705-15DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 13 01:57:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 13 01:54:07 2019
Response via : Initial Calibration

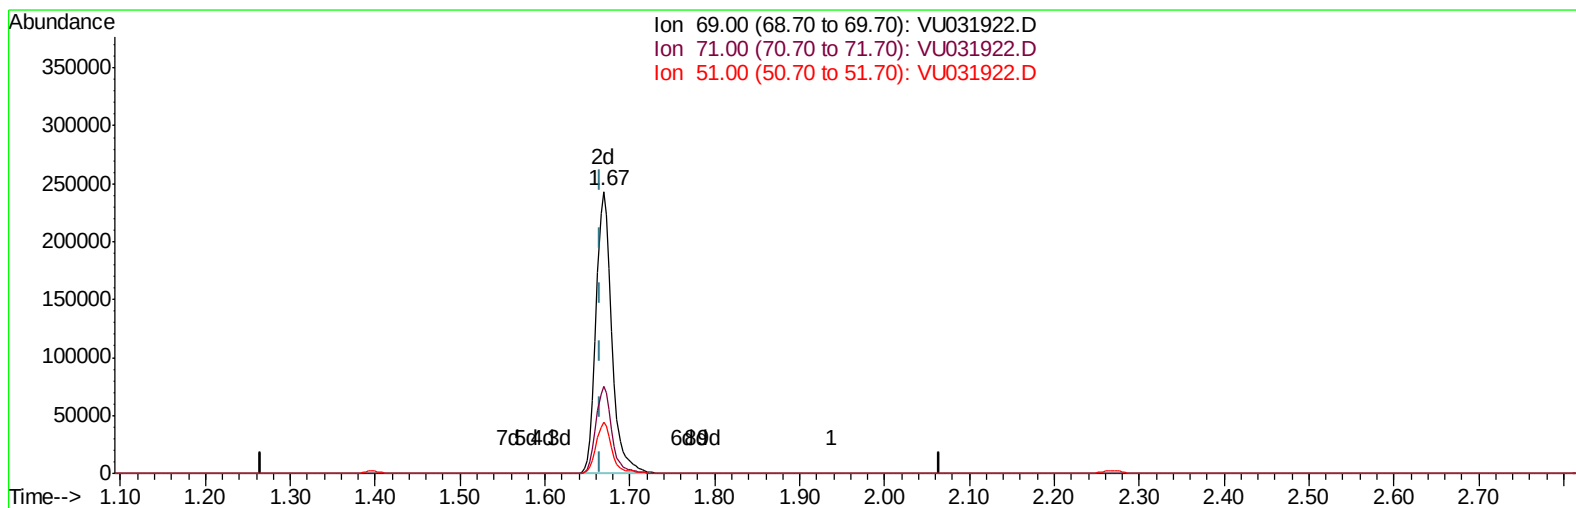

TIC: VU031922.D

(7) Chloroethane-d5 (S)

1.669min (+0.003) 47.30ug/L m

response 312526

Ion	Exp%	Act%
69.00	100	100
71.00	32.30	0.02#
51.00	29.10	0.02#
0.00	0.00	0.00