
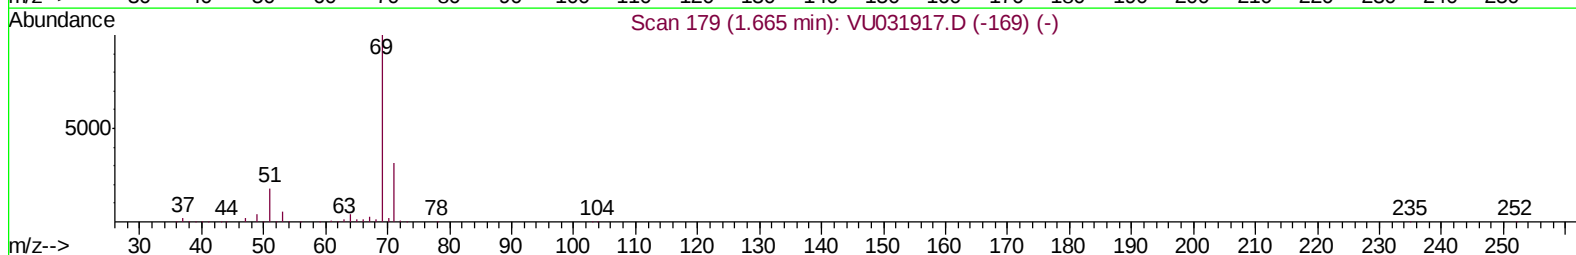
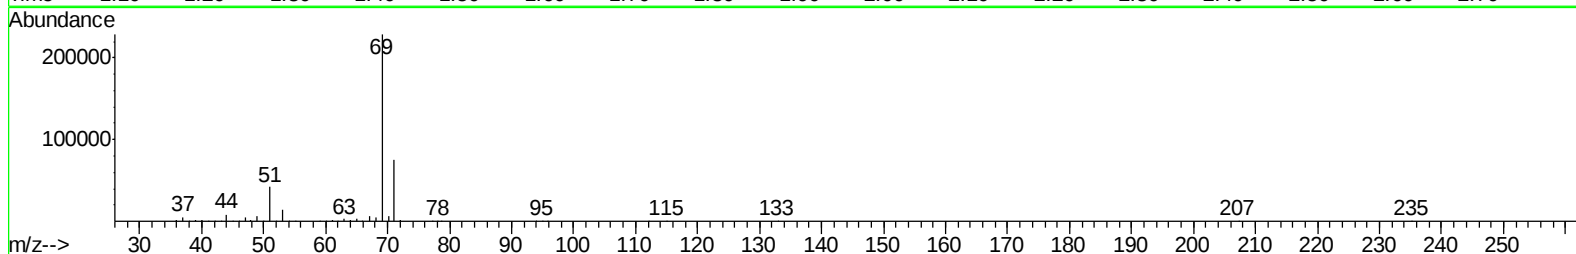


Data File : VU031923.D
Acq On : 11 May 2019 12:05
Operator : JC/SP
Sample : K2814-02 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 13 01:57:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 13 01:54:07 2019
Response via : Initial Calibration

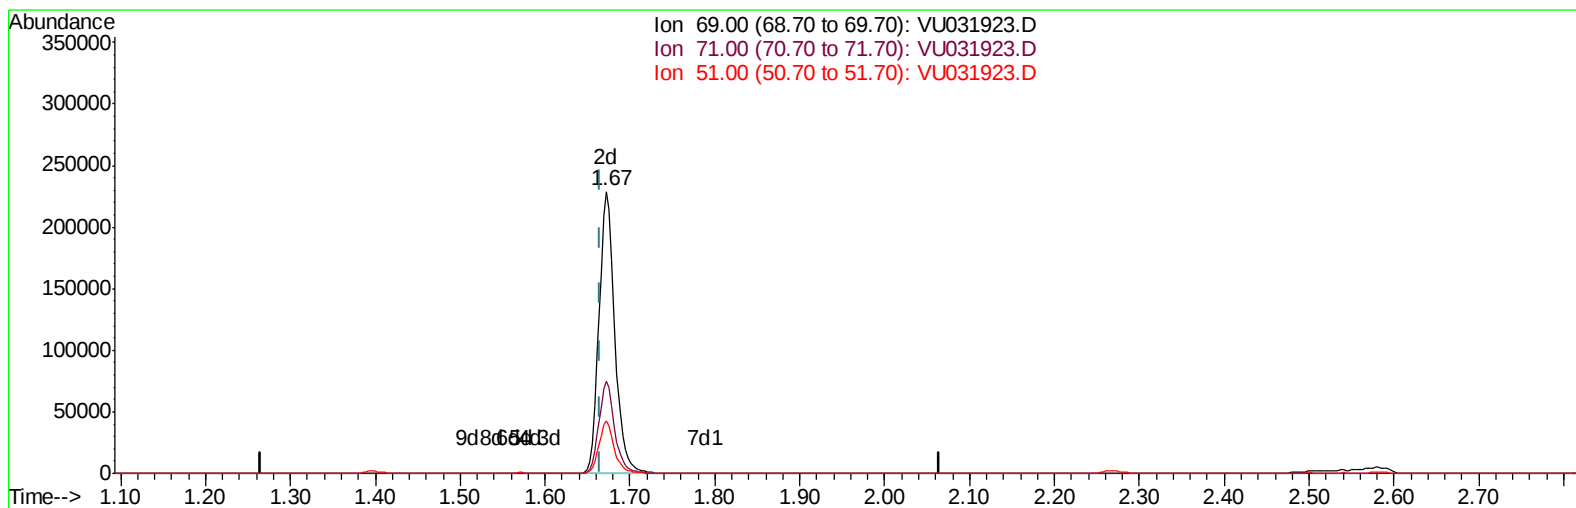

TIC: VU031923.D

(7) Chloroethane-d5 (S)

1.672min (+0.006) 44.44ug/L m

response 294886

Ion	Exp%	Act%
69.00	100	100
71.00	32.30	0.02#
51.00	29.10	0.01#
0.00	0.00	0.00