
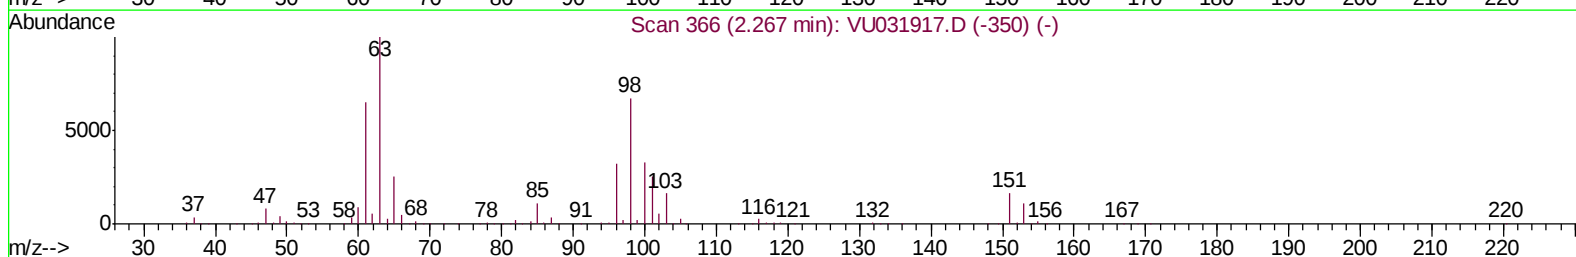
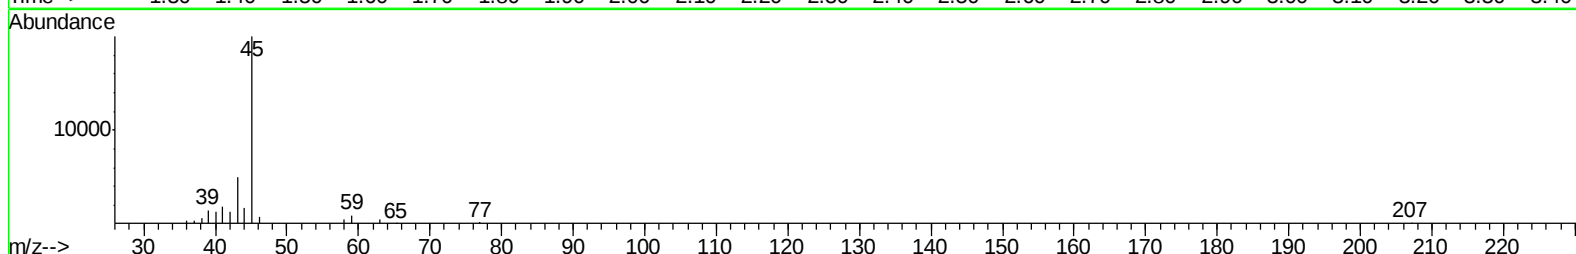


Data File : VU031926.D
Acq On : 11 May 2019 13:16
Operator : JC/SP
Sample : K2705-16DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: May 13 01:58:02 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 13 01:54:07 2019
Response via : Initial Calibration

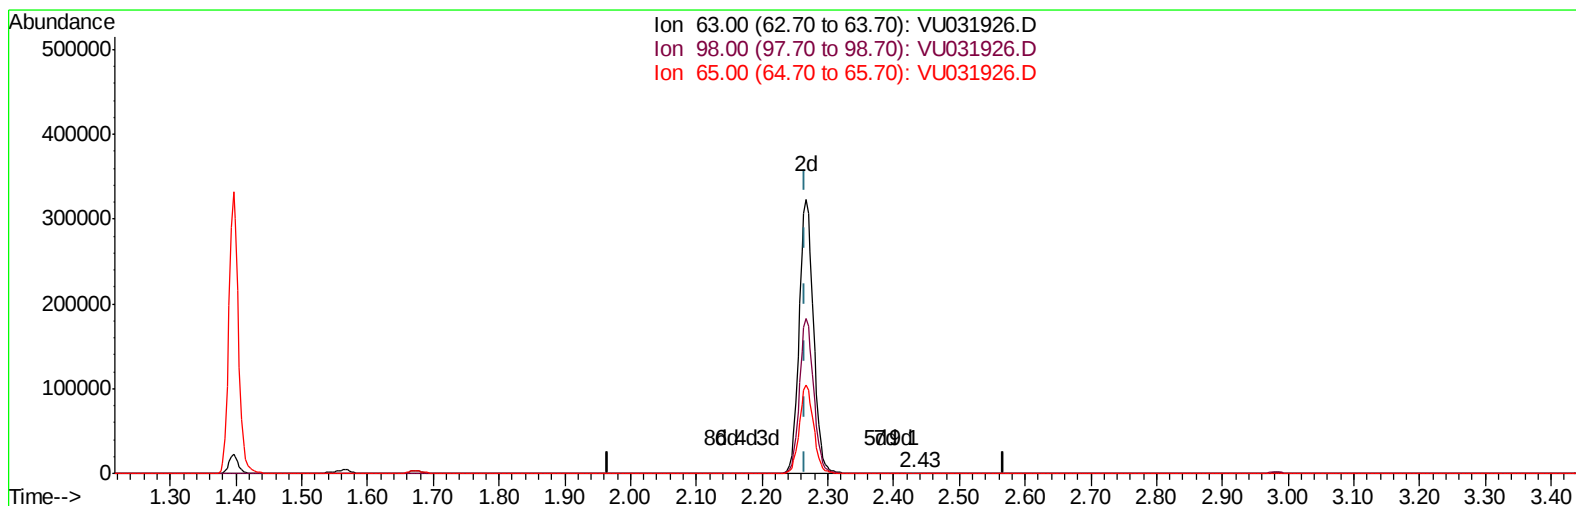

TIC: VU031926.D

(11) 1,1-Dichloroethene-d2 (S)

2.431min (+0.164) 0.01ug/L

response 152

Ion	Exp%	Act%
63.00	100	100
98.00	66.60	60.53
65.00	23.40	26.97
0.00	0.00	0.00