
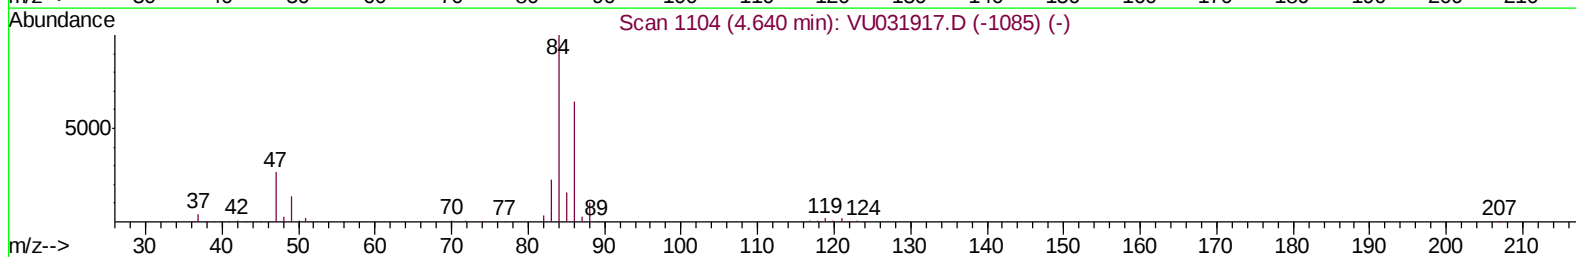
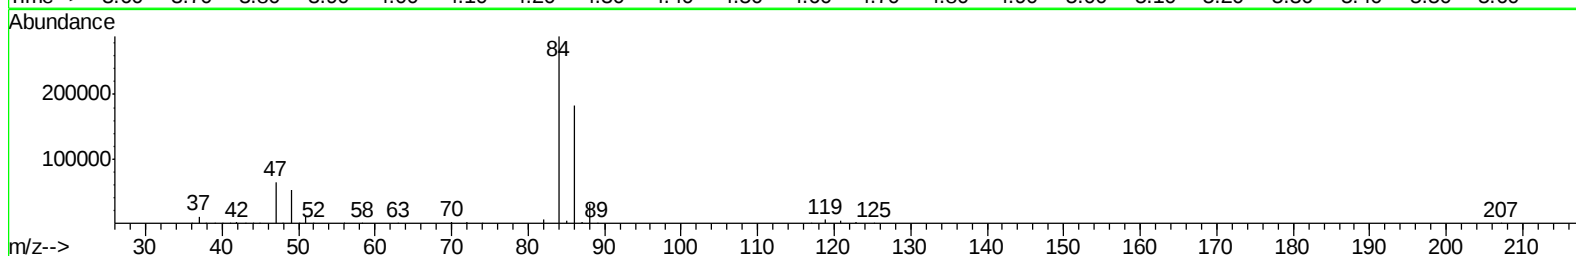


Data File : VU031929.D
Acq On : 11 May 2019 14:26
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 13 01:58:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 13 01:54:07 2019
Response via : Initial Calibration

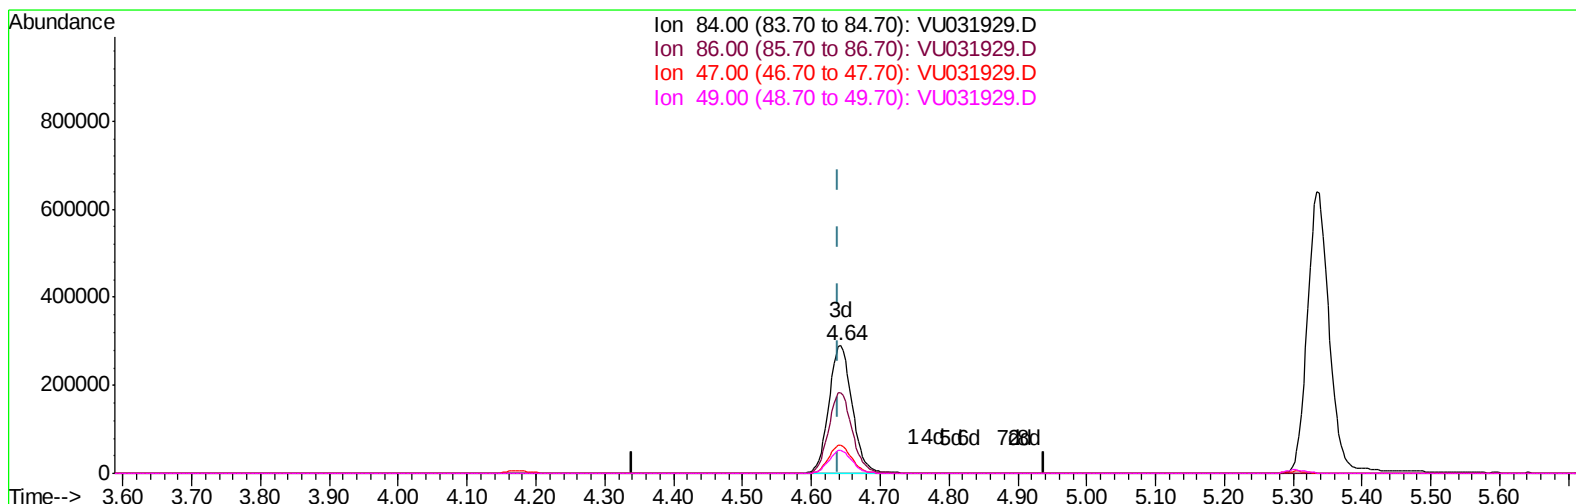

TIC: VU031929.D

(24) Chloroform-d (S)

4.643min (+0.003) 44.60ug/L m

response 683673

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	0.08#
47.00	45.70	0.05#
49.00	27.20	0.04#