

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051119\
 Data File : VU031929.D
 Acq On : 11 May 2019 14:26
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	105	rBV	583959	607378	14.42%	1.931%
2	1.672	173	181	199	rVB	441547	590966	14.03%	1.879%
3	2.267	355	366	379	rBV	925298	1395387	33.13%	4.436%
4	2.447	414	422	436	rBV	20153	36759	0.87%	0.117%
5	2.527	444	447	450	rBV4	1333	794	0.02%	0.003%
6	2.691	493	498	507	rVB4	2672	4046	0.10%	0.013%
7	2.829	534	541	546	rBV7	2216	3245	0.08%	0.010%
8	3.029	599	603	606	rBV3	959	720	0.02%	0.002%
9	3.074	615	617	622	rVB2	1685	886	0.02%	0.003%
10	3.106	622	627	629	rBV4	835	646	0.02%	0.002%
11	3.122	629	632	636	rVB3	1504	982	0.02%	0.003%
12	3.154	636	642	645	rBV2	973	902	0.02%	0.003%
13	3.170	645	647	652	rBV2	820	738	0.02%	0.002%
14	3.235	664	667	670	rVB	1264	796	0.02%	0.003%
15	3.286	679	683	684	rBV	741	523	0.01%	0.002%
16	3.360	701	706	708	rBV3	1406	1291	0.03%	0.004%
17	3.376	708	711	713	rVV	1030	813	0.02%	0.003%
18	3.399	715	718	721	rVV3	1655	1064	0.03%	0.003%
19	3.617	783	786	789	rBV3	924	618	0.01%	0.002%
20	3.739	821	824	828	rVB2	783	721	0.02%	0.002%
21	3.778	831	836	837	rBV	765	593	0.01%	0.002%
22	3.842	853	856	858	rVV2	942	716	0.02%	0.002%
23	3.913	873	878	884	rVV3	1251	1078	0.03%	0.003%
24	4.019	904	911	912	rBV2	1128	1271	0.03%	0.004%
25	4.064	923	925	935	rVB3	925	1214	0.03%	0.004%
26	4.106	935	938	941	rBV3	756	686	0.02%	0.002%
27	4.170	946	958	997	rBV	403235	1120788	26.61%	3.563%
28	4.643	1087	1105	1135	rBV	677425	1611962	38.27%	5.125%
29	4.945	1197	1199	1201	rBV2	1059	632	0.02%	0.002%
30	5.048	1227	1231	1235	rVB3	1769	1395	0.03%	0.004%
31	5.115	1249	1252	1255	rBV3	815	553	0.01%	0.002%
32	5.148	1259	1262	1266	rBV4	767	568	0.01%	0.002%
33	5.206	1276	1280	1283	rBV3	1016	811	0.02%	0.003%
34	5.334	1292	1320	1365	rBV2	1389190	4211637	100.00%	13.389%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U051119\
 Data File : VU031929.D
 Acq On : 11 May 2019 14:26
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.771	1453	1456	1459	rBV2	1000	737	0.02%	0.002%
36	5.881	1476	1490	1535	rBV	1193929	2517689	59.78%	8.004%
37	6.180	1577	1583	1605	rVB10	24207	55829	1.33%	0.177%
38	6.324	1615	1628	1658	rBV	940398	1914293	45.45%	6.086%
39	6.559	1699	1701	1704	rVB3	2094	1136	0.03%	0.004%
40	6.636	1722	1725	1727	rBV4	818	609	0.01%	0.002%
41	6.649	1727	1729	1733	rVV4	777	538	0.01%	0.002%
42	6.778	1766	1769	1772	rVB2	1319	787	0.02%	0.003%
43	6.820	1779	1782	1783	rBV	1041	549	0.01%	0.002%
44	6.881	1799	1801	1805	rBV3	830	567	0.01%	0.002%
45	7.003	1833	1839	1842	rBV5	884	1114	0.03%	0.004%
46	7.103	1868	1870	1876	rVB4	1049	702	0.02%	0.002%
47	7.148	1882	1884	1887	rVB3	930	502	0.01%	0.002%
48	7.225	1895	1908	1935	rBV	470237	869058	20.63%	2.763%
49	7.492	1987	1991	1995	rBV4	987	1128	0.03%	0.004%
50	7.562	2000	2013	2036	rBV	1677532	3097973	73.56%	9.849%
51	7.848	2091	2102	2132	rBV	317640	579661	13.76%	1.843%
52	8.122	2185	2187	2192	rVB2	1474	1029	0.02%	0.003%
53	8.148	2192	2195	2196	rBV3	1119	548	0.01%	0.002%
54	8.180	2196	2205	2208	rVV10	2730	3243	0.08%	0.010%
55	8.228	2215	2220	2230	rVB7	5564	9193	0.22%	0.029%
56	8.308	2233	2245	2291	rBV	1254078	2471525	58.68%	7.857%
57	8.739	2376	2379	2384	rBV4	1387	1206	0.03%	0.004%
58	8.810	2399	2401	2403	rBV3	1034	585	0.01%	0.002%
59	8.836	2407	2409	2414	rVB3	1693	1261	0.03%	0.004%
60	9.086	2474	2487	2531	rVV	1790181	3191669	75.78%	10.146%
61	9.414	2586	2589	2593	rVB5	1100	595	0.01%	0.002%
62	9.459	2600	2603	2607	rVB4	1687	1235	0.03%	0.004%
63	9.488	2607	2612	2614	rBV4	2131	1920	0.05%	0.006%
64	9.533	2621	2626	2628	rBV4	1160	1212	0.03%	0.004%
65	9.604	2644	2648	2652	rBV3	1126	955	0.02%	0.003%
66	9.691	2671	2675	2678	rBV4	862	772	0.02%	0.002%
67	9.723	2682	2685	2688	rVV2	794	541	0.01%	0.002%
68	9.778	2700	2702	2706	rVB2	1271	731	0.02%	0.002%
69	9.861	2725	2728	2732	rBV3	969	648	0.02%	0.002%
70	9.935	2748	2751	2754	rVB	1043	674	0.02%	0.002%
71	9.958	2754	2758	2759	rBV2	659	481	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051119\
 Data File : VU031929.D
 Acq On : 11 May 2019 14:26
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.016	2773	2776	2781	rVV3	1088	788	0.02%	0.003%
73	10.045	2783	2785	2793	rVB4	1366	1184	0.03%	0.004%
74	10.090	2797	2799	2804	rVV4	849	471	0.01%	0.001%
75	10.154	2814	2819	2822	rBV3	1152	1301	0.03%	0.004%
76	10.225	2835	2841	2846	rBV8	1054	1259	0.03%	0.004%
77	10.282	2857	2859	2862	rVB3	916	494	0.01%	0.002%
78	10.427	2890	2904	2929	rBV	1308726	2122229	50.39%	6.747%
79	10.668	2977	2979	2983	rVB4	1121	749	0.02%	0.002%
80	10.742	3000	3002	3009	rVB3	1268	1299	0.03%	0.004%
81	10.771	3009	3011	3013	rBV3	868	485	0.01%	0.002%
82	10.874	3039	3043	3048	rVB4	817	837	0.02%	0.003%
83	11.096	3109	3112	3115	rVB3	2312	1477	0.04%	0.005%
84	11.118	3115	3119	3120	rBV	904	611	0.01%	0.002%
85	11.170	3130	3135	3141	rBV6	1232	1439	0.03%	0.005%
86	11.196	3141	3143	3151	rVV5	929	905	0.02%	0.003%
87	11.231	3151	3154	3160	rVB4	980	953	0.02%	0.003%
88	11.318	3178	3181	3185	rBV2	1129	883	0.02%	0.003%
89	11.385	3199	3202	3205	rVB4	998	639	0.02%	0.002%
90	11.411	3205	3210	3212	rBV3	844	740	0.02%	0.002%
91	11.479	3218	3231	3255	rBV	1480208	2431611	57.74%	7.730%
92	11.855	3335	3348	3366	rBV	1528875	2542541	60.37%	8.083%
93	12.733	3619	3621	3622	rBV2	1119	529	0.01%	0.002%
94	12.932	3681	3683	3684	rBV2	1416	639	0.02%	0.002%
95	13.369	3817	3819	3824	rBV2	1115	796	0.02%	0.003%
96	13.549	3873	3875	3878	rBV	1142	637	0.02%	0.002%
97	13.585	3882	3886	3887	rBV2	939	619	0.01%	0.002%
98	13.945	3995	3998	4003	rBV4	1450	1061	0.03%	0.003%
99	14.025	4019	4023	4024	rBV2	1388	989	0.02%	0.003%
100	14.212	4077	4081	4084	rBV4	1671	1746	0.04%	0.006%


Sum of corrected areas: 31455985

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051119\
Data File : VU031929.D
Acq On : 11 May 2019 14:26
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

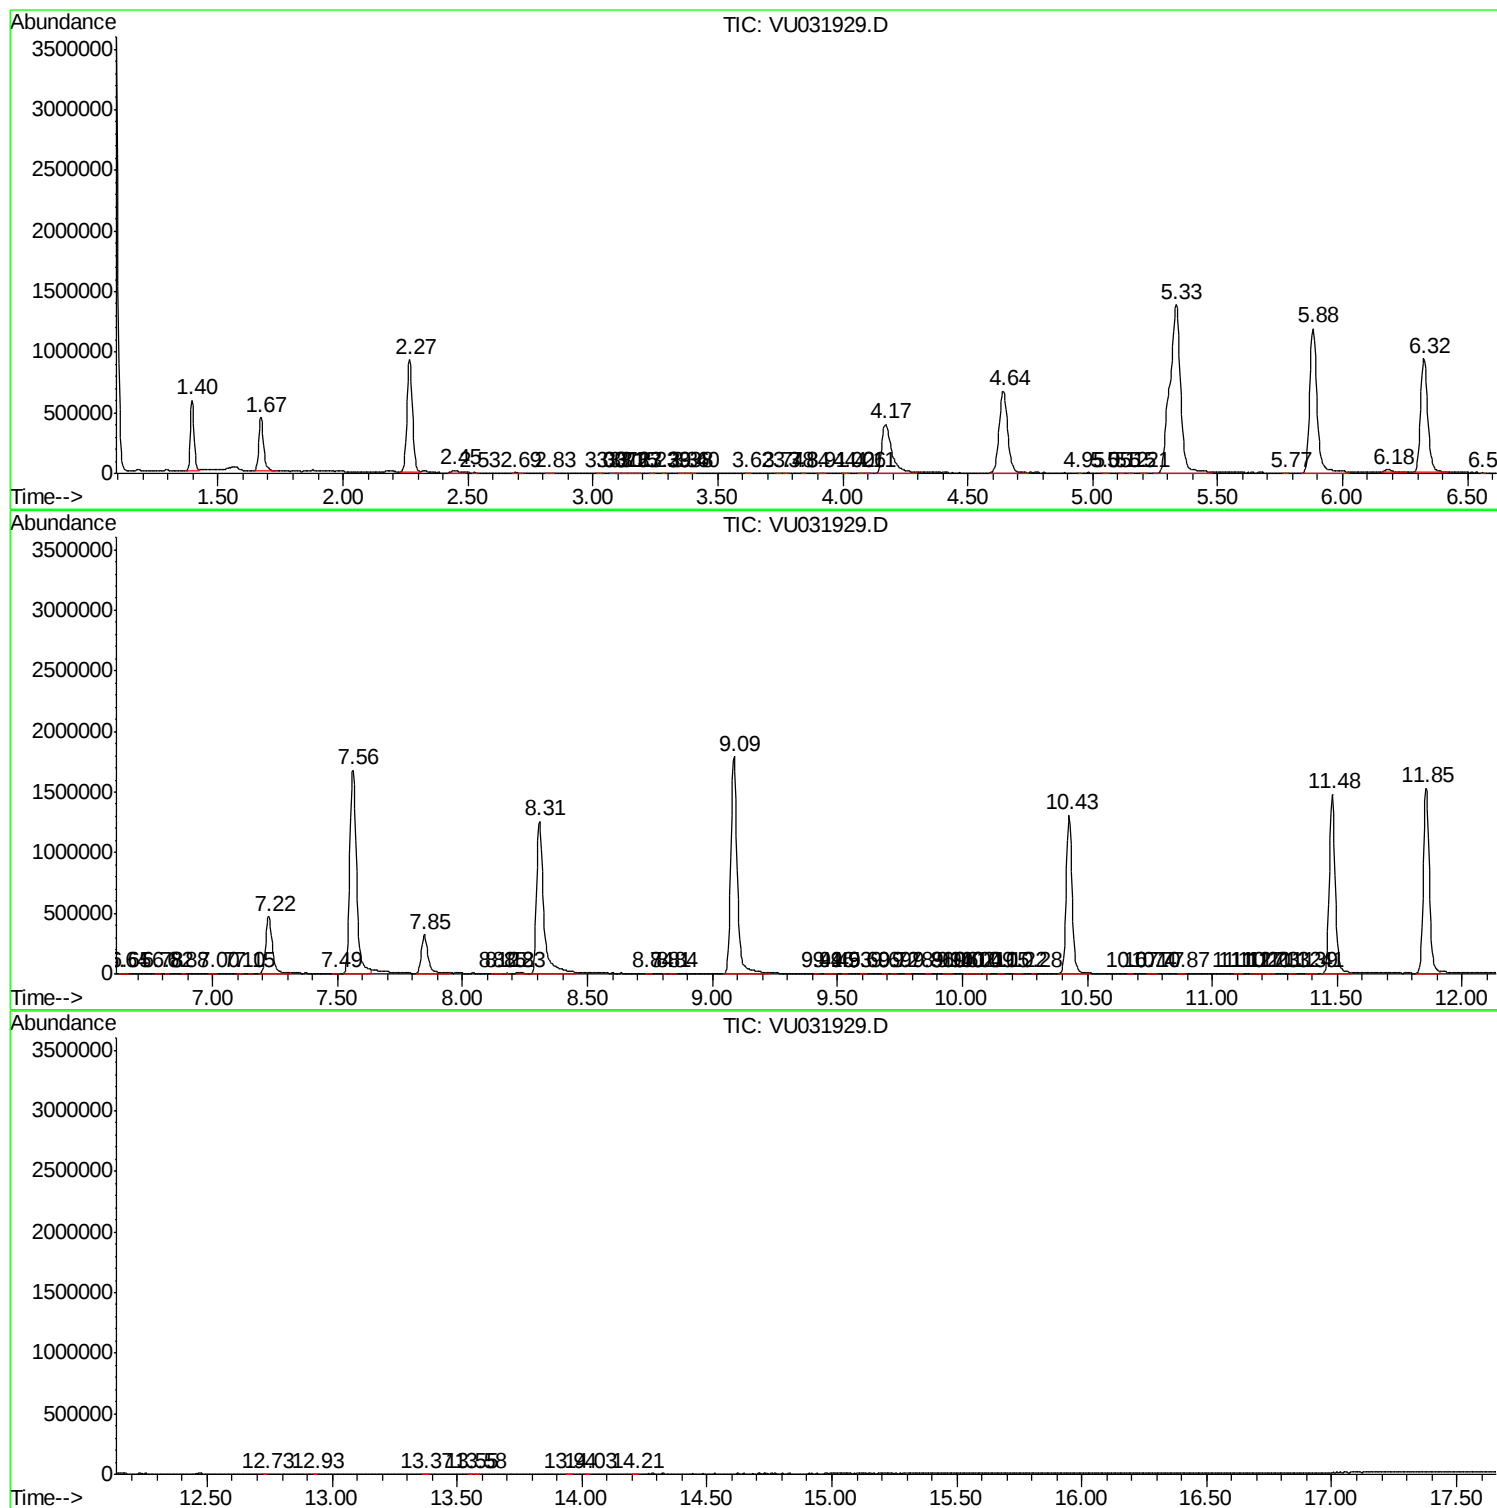

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051119\
Data File : VU031929.D
Acq On : 11 May 2019 14:26
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051119\
Data File : VU031929.D
Acq On : 11 May 2019 14:26
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc