


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051119\
 Data File : VU031916.D
 Acq On : 11 May 2019 09:11
 Operator : JC/SP
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Mon May 13 01:54:07 2019

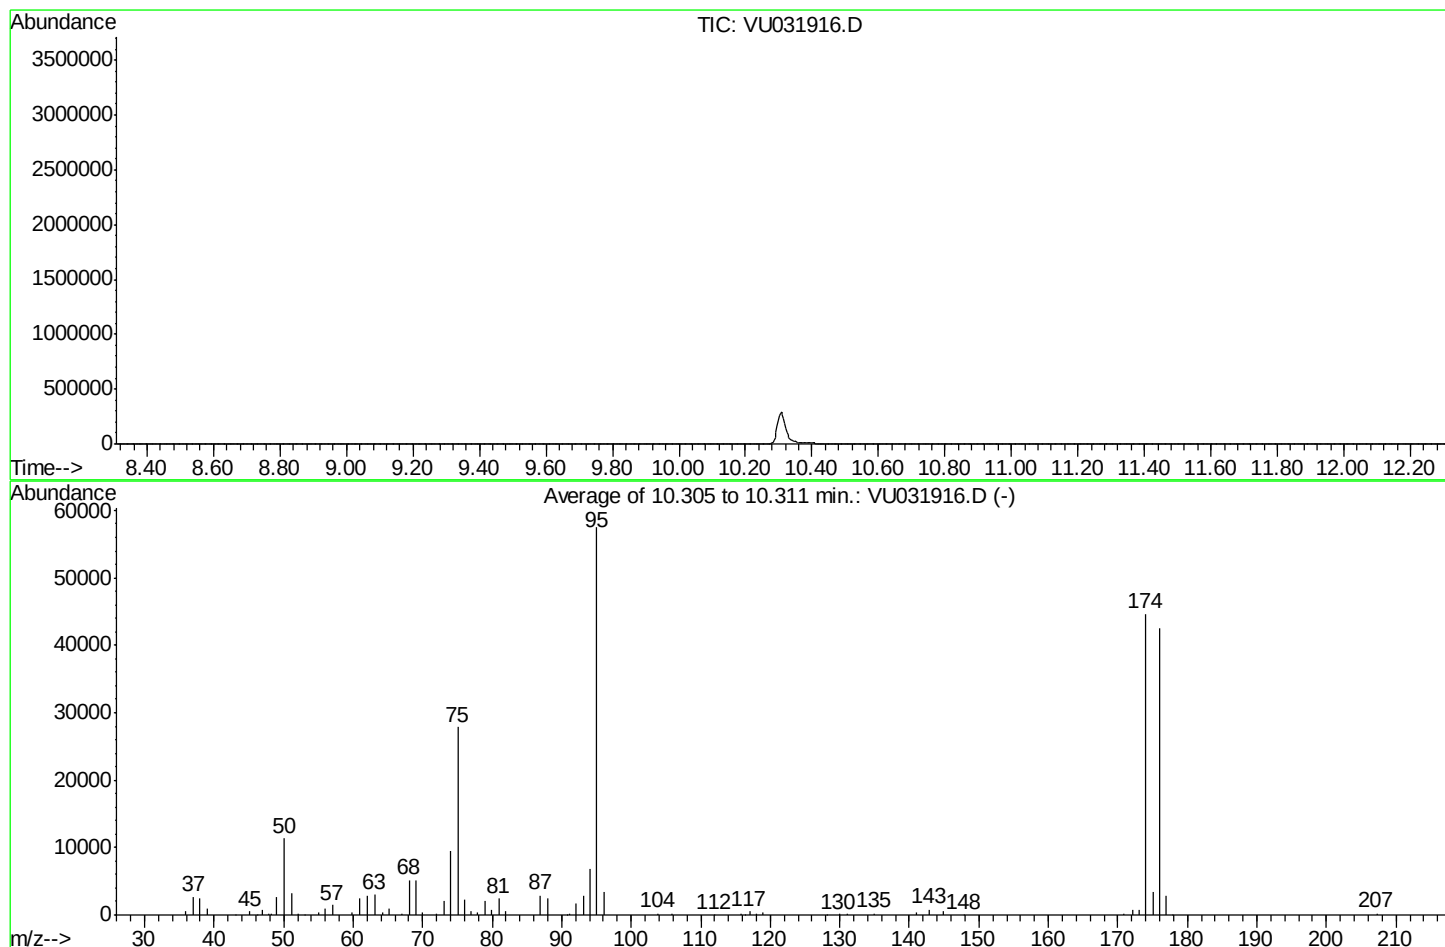

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	11309	PASS
75	95	30	80	48.5	27896	PASS
95	95	100	100	100.0	57488	PASS
96	95	5	9	6.0	3437	PASS
173	174	0.00	2	1.7	771	PASS
174	95	50	120	77.6	44637	PASS
175	174	5	9	7.6	3401	PASS
176	174	95	101	95.2	42506	PASS
177	176	5	9	6.6	2818	PASS

Scan 2854 (10.266 min): VU031916.D
BFB41

m/z	Abundance
40.00	1237.0
44.00	1375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	641.0
37.00	2730.0
38.00	2711.0
39.00	1061.0
39.90	1044.0
44.10	1262.0
45.10	661.0
46.20	137.0
47.00	859.0
47.90	394.0
49.00	2408.0
50.10	11559.0
51.10	3448.0
52.10	194.0
53.00	160.0
55.10	290.0
56.00	954.0
57.00	1549.0
59.90	632.0
61.00	2579.0
62.10	2886.0
63.10	3186.0
64.20	556.0
65.10	905.0
66.90	164.0
68.00	5521.0
69.00	5282.0
70.10	324.0
71.90	319.0
73.10	2323.0
74.10	9980.0
75.00	28216.0
76.00	2349.0
76.90	457.0
77.90	324.0
78.90	1978.0
79.90	746.0
81.00	2567.0
81.90	452.0
87.00	3397.0
88.00	2551.0
90.80	168.0
92.00	1555.0
93.10	2682.0
94.10	7022.0
95.10	58632.0
96.10	3538.0
103.90	244.0
105.90	265.0
115.80	141.0
116.30	153.0
117.10	506.0
118.00	214.0
118.90	421.0
128.10	134.0
129.90	112.0
131.10	185.0
135.00	202.0
140.90	463.0
142.90	788.0
144.90	422.0
170.90	189.0
172.10	829.0
173.00	757.0
174.00	42776.0
175.00	3410.0
176.00	42400.0
177.00	2715.0
177.90	116.0
207.20	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	647.0
37.00	2829.0
38.00	2583.0
39.00	902.0
39.90	1106.0
43.10	107.0
44.00	1309.0
45.10	593.0
47.00	710.0
47.70	316.0
48.20	307.0
49.00	2739.0
50.10	11448.0
51.10	3371.0
52.10	174.0
53.00	142.0
55.00	339.0
56.00	1016.0
57.00	1556.0
59.90	441.0
61.00	2414.0
62.10	2985.0
63.10	3037.0
64.20	418.0
65.10	950.0
67.00	165.0
68.10	5423.0
69.00	5401.0
70.00	314.0
71.90	252.0
73.10	2193.0
74.00	9562.0
75.10	28704.0
76.10	2290.0
76.90	523.0
77.90	336.0
78.90	2177.0
79.90	703.0
81.00	2538.0
81.90	615.0
87.00	3076.0
88.00	2544.0
91.10	229.0
92.00	1692.0
93.10	2999.0
94.10	7047.0
95.10	58896.0
96.10	3498.0
103.90	267.0
105.90	196.0
112.00	127.0
115.70	163.0
117.10	564.0
117.90	269.0
118.90	401.0
129.90	146.0
131.20	192.0
135.00	218.0
140.90	442.0
143.00	800.0
144.90	555.0
147.90	101.0
170.90	192.0
172.10	895.0
173.00	809.0
174.00	46088.0
175.00	3544.0
176.00	43968.0
177.00	2946.0
177.90	104.0
207.20	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	540.0
37.10	2675.0
38.00	2344.0
39.00	854.0
39.90	1119.0
43.10	120.0
44.00	1391.0
45.10	447.0
47.00	548.0
48.20	344.0
49.00	2820.0
50.10	10922.0
51.10	3161.0
52.10	171.0
55.00	348.0
56.00	856.0
57.00	1436.0
59.90	339.0
61.00	2269.0
62.10	2608.0
63.10	2709.0
64.00	401.0
65.10	838.0
67.00	174.0
68.10	4718.0
69.00	4965.0
69.90	324.0
71.90	203.0
73.00	1997.0
74.00	9009.0
75.10	26768.0
76.10	2128.0
76.90	471.0
77.80	281.0
78.90	2281.0
80.00	615.0
80.90	2158.0
82.00	585.0
86.90	2374.0
88.00	2303.0
91.10	319.0
92.10	1703.0
93.10	2778.0
94.10	6398.0
95.00	54936.0
96.00	3275.0
103.90	251.0
105.80	176.0
111.90	121.0
115.70	152.0
117.00	552.0
117.90	255.0
118.90	299.0
130.00	189.0
131.10	124.0
134.90	173.0
141.00	447.0
143.00	738.0
144.90	593.0
147.90	108.0
170.90	119.0
172.10	779.0
173.10	747.0
174.00	45048.0
175.00	3249.0
176.00	41152.0
177.00	2794.0
207.30	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41