

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051120\
Data File : VU038109.D
Acq On : 11 May 2020 16:20
Operator : JC/MD
Sample : L2578-02DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSF1DL

Manual Integrations
APPROVED

sam
5/12/2020 3:21:59 PM

Quant Time: May 12 01:13:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 12 01:10:23 2020
Response via : Initial Calibration

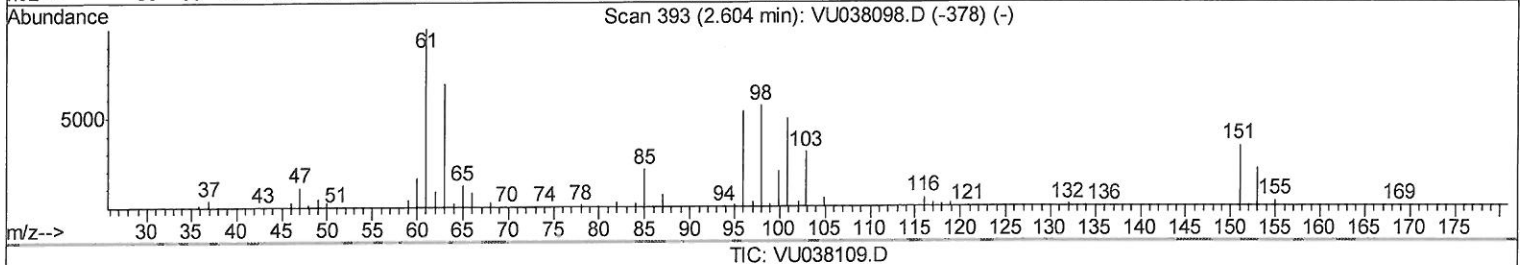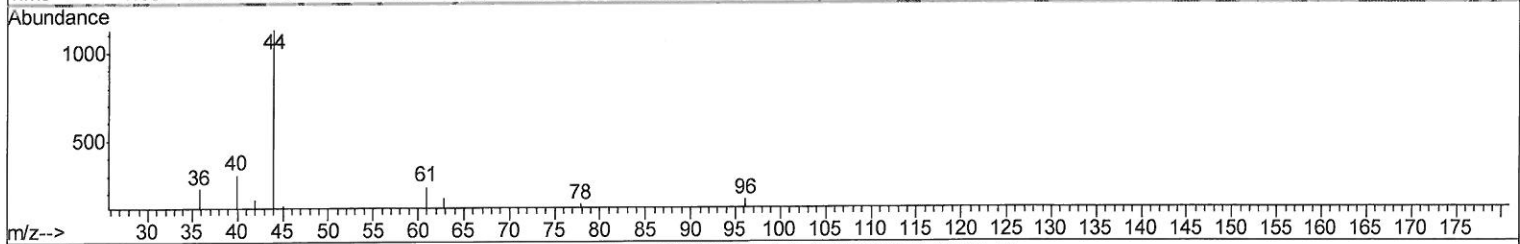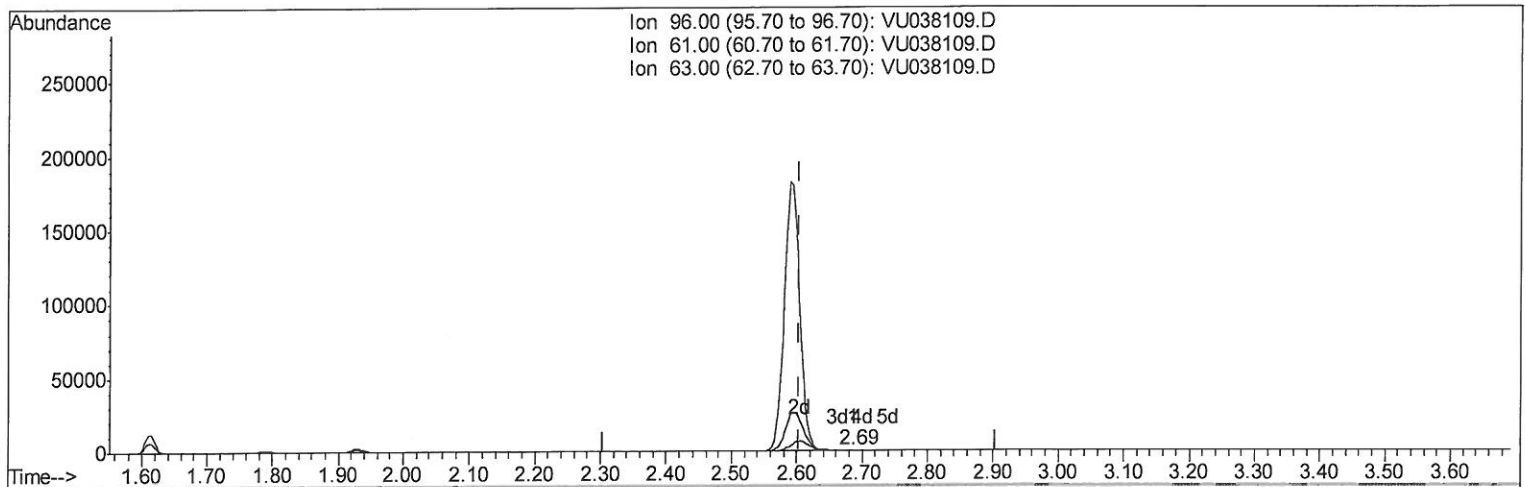

(12) 1,1-Dichloroethene (T)

2.687min (+0.084) 0.03ug/L

response 130

Ion	Exp%	Act%
96.00	100	100
61.00	180.20	143.90
63.00	119.10	104.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051120\
 Data File : VU038109.D
 Acq On : 11 May 2020 16:20
 Operator : JC/MD
 Sample : L2578-02DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSF1DL

Manual Integrations
 APPROVED

sam
 5/12/2020 3:21:59 PM

Quant Time: May 12 01:13:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 12 01:10:23 2020
 Response via : Initial Calibration

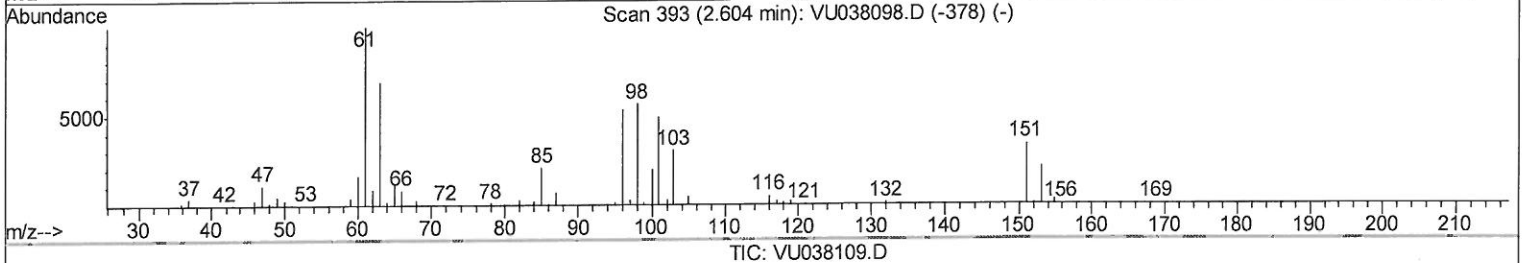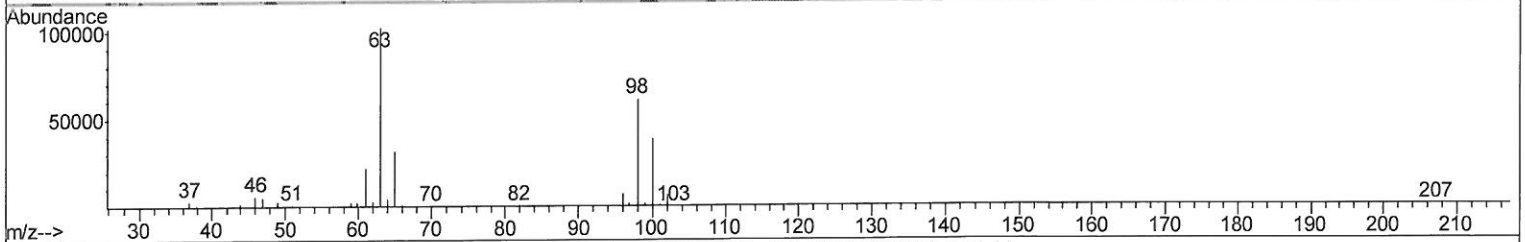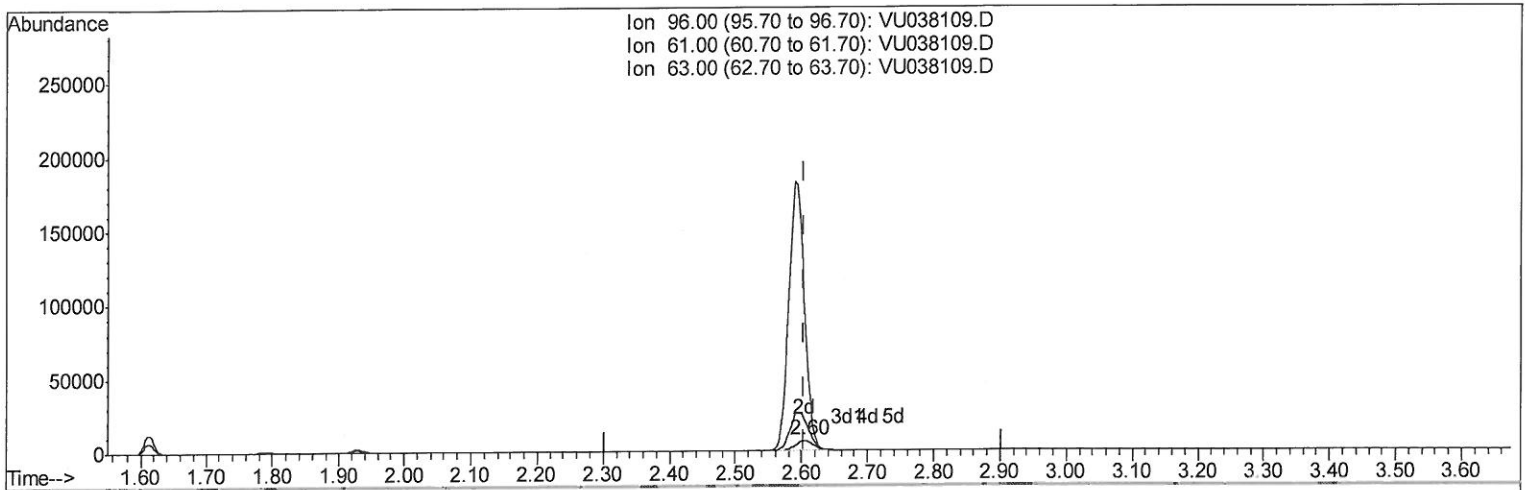

(12) 1,1-Dichloroethene (T)

2.604min (-0.000) 2.52ug/L m

response 13014

Ion	Exp%	Act%
96.00	100	100
61.00	180.20	311.54#
63.00	119.10	1480.09#
0.00	0.00	0.00

05/12/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051120\
 Data File : VU038109.D
 Acq On : 11 May 2020 16:20
 Operator : JC/MD
 Sample : L2578-02DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sample ID :
 BFSF1DL

Manual Integrations
 APPROVED

sam
 5/12/2020 3:21:59 PM

Quant Time: May 12 03:10:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 12 01:10:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	787394	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	758137	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	363981	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	215127	31.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	62.12%
7) Chloroethane-d5	1.93	69	207574	36.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	73.68%
11) 1,1-Dichloroethene-d2	2.59	63	297728	26.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	52.56%#
21) 2-Butanone-d5	4.66	46	508553	93.95	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.95%
24) Chloroform-d	5.10	84	416480	38.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.66%
26) 1,2-Dichloroethane-d4	5.74	65	295410	39.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.30%
32) Benzene-d6	5.76	84	885504	39.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.26%
36) 1,2-Dichloropropane-d6	6.72	67	305177	41.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.38%
41) Toluene-d8	7.92	98	784814	38.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.58%#
43) trans-1,3-Dichloropropene-	8.20	79	134453	38.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.40%
47) 2-Hexanone-d5	8.65	63	338882	105.17	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.17%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	443917	41.58	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.16%
64) 1,2-Dichlorobenzene-d4	12.20	152	306542	40.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.56%

Target Compounds

12) 1,1-Dichloroethene	2.60	96	13014m	2.524	ug/L	99
19) 1,1-Dichloroethane	3.91	63	210924	19.017	ug/L	99
30) 1,1,1-Trichloroethane	5.35	97	537680	63.803	ug/L #	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051120\
Data File : VU038109.D
Acq On : 11 May 2020 16:20
Operator : JC/MD
Sample : L2578-02DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleID :
BFSF1DL

Manual Integrations
APPROVED

sam
5/12/2020 3:21:59 PM

Quant Time: May 12 03:10:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 12 01:10:23 2020
Response via : Initial Calibration

