


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051120\
 Data File : VU038097.D
 Acq On : 11 May 2020 09:18
 Operator : JC/MD
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis
 Last Update : Tue May 12 01:10:23 2020

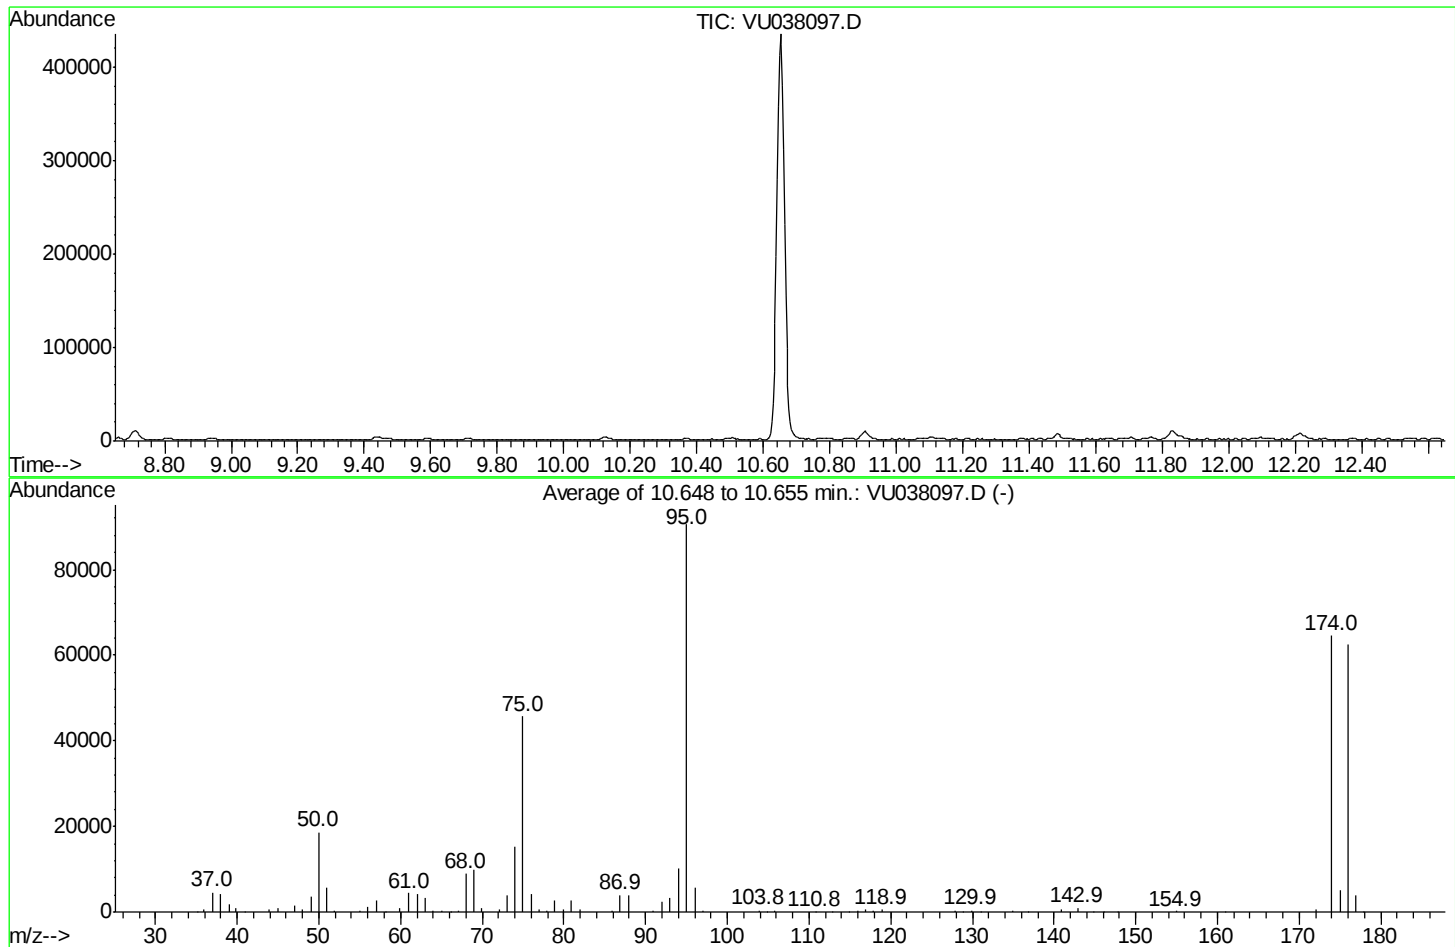

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	18624	PASS
75	95	30	80	50.5	45736	PASS
95	95	100	100	100.0	90578	PASS
96	95	5	9	6.4	5795	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.2	64474	PASS
175	174	5	9	7.7	4974	PASS
176	174	95	101	96.8	62389	PASS
177	176	5	9	6.2	3895	PASS

m/z	Abundance
35.90	367.0
38.10	171.0
39.90	318.0
43.90	936.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	1017.0
37.00	4456.0
38.00	4445.0
39.10	1817.0
39.90	1323.0
43.90	1476.0
45.00	822.0
47.00	1365.0
47.90	642.0
49.00	3285.0
50.00	18208.0
51.00	5714.0
52.00	247.0
55.10	244.0
55.90	1196.0
57.00	2769.0
59.90	781.0
61.00	4261.0
62.00	4473.0
63.00	3157.0
64.00	345.0
65.10	335.0
67.10	306.0
68.00	8581.0
69.00	9675.0
69.90	792.0
72.00	529.0
73.00	3848.0
74.00	14921.0
75.00	44616.0
76.00	4150.0
77.00	704.0
78.00	329.0
78.90	2646.0
79.90	543.0
80.90	2586.0
81.90	622.0
85.80	224.0
86.90	3908.0
88.00	3774.0
90.90	339.0
92.00	2334.0
93.00	3342.0
94.00	10292.0
95.00	88496.0
96.00	6044.0
96.90	175.0
103.80	409.0
104.80	112.0
105.80	247.0
114.90	160.0
115.90	282.0
117.00	435.0
117.80	235.0
118.90	550.0
128.00	262.0
129.00	102.0
129.90	322.0
130.90	144.0
135.00	164.0
140.90	770.0
142.90	921.0
146.00	102.0
147.80	175.0
155.00	172.0
172.00	578.0
174.00	61768.0
175.00	5039.0
176.00	59352.0
177.00	3834.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.10	160.0
36.00	1029.0
37.00	4705.0
38.00	4538.0
39.00	1814.0
39.90	1265.0
40.90	101.0
43.90	1564.0
45.00	829.0
47.00	1446.0
47.90	615.0
49.00	3533.0
50.00	19160.0
51.00	5889.0
51.90	217.0
55.00	346.0
56.00	1265.0
57.00	2712.0
58.20	110.0
60.00	866.0
61.00	4623.0
62.00	4380.0
63.00	3219.0
64.00	378.0
65.10	318.0
68.00	9144.0
69.00	10216.0
70.00	793.0
72.10	628.0
73.00	4122.0
74.00	15726.0
75.00	46808.0
76.00	4330.0
77.00	655.0
77.90	389.0
78.90	2737.0
79.90	594.0
80.90	2584.0
81.90	648.0
85.90	263.0
86.90	4109.0
88.00	3944.0
90.90	357.0
92.00	2577.0
93.00	3493.0
94.00	10597.0
95.00	93200.0
96.00	5896.0
97.00	197.0
103.80	438.0
104.80	150.0
105.90	360.0
112.80	122.0
114.90	150.0
115.90	310.0
117.00	519.0
117.90	267.0
118.90	576.0
127.90	275.0
128.90	127.0
129.90	383.0
130.90	120.0
134.90	190.0
136.80	100.0
140.90	741.0
142.90	930.0
144.80	102.0
146.00	136.0
147.80	147.0
154.90	243.0
161.00	102.0
172.00	566.0
174.00	65952.0
175.00	5137.0
176.00	64120.0
177.00	3966.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.10	130.0
36.00	1072.0
37.00	4625.0
38.00	4298.0
39.00	1758.0
39.90	1103.0
43.90	1568.0
45.00	767.0
47.00	1365.0
47.90	521.0
49.00	3580.0
50.00	18504.0
51.00	5575.0
51.90	229.0
55.00	431.0
56.00	1327.0
57.00	2381.0
58.20	124.0
60.00	839.0
61.00	4545.0
62.00	4054.0
63.00	3223.0
64.00	403.0
65.00	317.0
66.20	113.0
66.90	183.0
68.00	8956.0
69.00	9823.0
70.00	790.0
72.10	519.0
73.00	4073.0
74.00	15208.0
75.00	45784.0
76.00	4032.0
76.90	600.0
77.90	460.0
78.90	2644.0
79.90	582.0
80.90	2521.0
81.90	597.0
85.90	231.0
86.90	3978.0
88.00	3663.0
90.80	266.0
92.00	2638.0
93.00	3285.0
94.00	10022.0
95.00	90040.0
96.00	5446.0
97.00	180.0
103.90	397.0
104.90	214.0
105.90	424.0
110.80	121.0
112.80	116.0
115.90	255.0
116.90	517.0
117.90	299.0
118.90	509.0
127.90	306.0
128.80	151.0
129.90	384.0
131.00	114.0
134.90	192.0
140.90	678.0
142.90	861.0
146.00	128.0
147.80	102.0
154.90	278.0
160.90	109.0
172.00	513.0
174.00	65704.0
175.00	4748.0
176.00	63696.0
177.00	3885.0
177.90	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48