

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU051121\  
 Data File : VU043656.D  
 Acq On : 11 May 2021 11:57  
 Operator : SY/MD  
 Sample : M2301-03  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BG6J3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043656.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.604       | 74            | 82          | 97           | rVB      | 39634          | 44381         | 8.61%           | 1.367%        |
| 2         | 1.919       | 172           | 180         | 193          | rVB      | 34601          | 45183         | 8.76%           | 1.392%        |
| 3         | 2.575       | 372           | 384         | 400          | rBV      | 72143          | 118000        | 22.89%          | 3.636%        |
| 4         | 3.883       | 775           | 791         | 803          | rVB4     | 2631           | 7154          | 1.39%           | 0.220%        |
| 5         | 4.645       | 1011          | 1028        | 1060         | rBV      | 50887          | 179121        | 34.74%          | 5.519%        |
| 6         | 5.073       | 1146          | 1161        | 1182         | rBV3     | 72960          | 182563        | 35.41%          | 5.625%        |
| 7         | 5.735       | 1342          | 1367        | 1389         | rBV3     | 132048         | 352009        | 68.28%          | 10.846%       |
| 8         | 6.256       | 1516          | 1529        | 1547         | rBV      | 128597         | 241031        | 46.75%          | 7.427%        |
| 9         | 6.549       | 1609          | 1620        | 1631         | rVB5     | 5427           | 9388          | 1.82%           | 0.289%        |
| 10        | 6.700       | 1654          | 1667        | 1684         | rBV      | 92428          | 177802        | 34.49%          | 5.479%        |
| 11        | 7.574       | 1927          | 1939        | 1965         | rBV      | 45206          | 79650         | 15.45%          | 2.454%        |
| 12        | 7.906       | 2029          | 2042        | 2057         | rBV      | 146235         | 249177        | 48.33%          | 7.678%        |
| 13        | 8.189       | 2118          | 2130        | 2144         | rBV2     | 28293          | 48804         | 9.47%           | 1.504%        |
| 14        | 8.558       | 2233          | 2245        | 2257         | rBV2     | 41826          | 70206         | 13.62%          | 2.163%        |
| 15        | 8.645       | 2258          | 2272        | 2303         | rBV      | 234407         | 515568        | 100.00%         | 15.886%       |
| 16        | 9.423       | 2501          | 2514        | 2534         | rBV      | 190219         | 310182        | 60.16%          | 9.557%        |
| 17        | 10.764      | 2920          | 2931        | 2945         | rVB      | 71219          | 115578        | 22.42%          | 3.561%        |
| 18        | 11.819      | 3248          | 3259        | 3274         | rBV      | 171018         | 267098        | 51.81%          | 8.230%        |
| 19        | 12.201      | 3366          | 3378        | 3392         | rBV      | 143504         | 232544        | 45.10%          | 7.165%        |


Sum of corrected areas: 3245439

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU051121\  
Data File : VU043656.D  
Acq On : 11 May 2021 11:57  
Operator : SY/MD  
Sample : M2301-03  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BG6J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR050321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

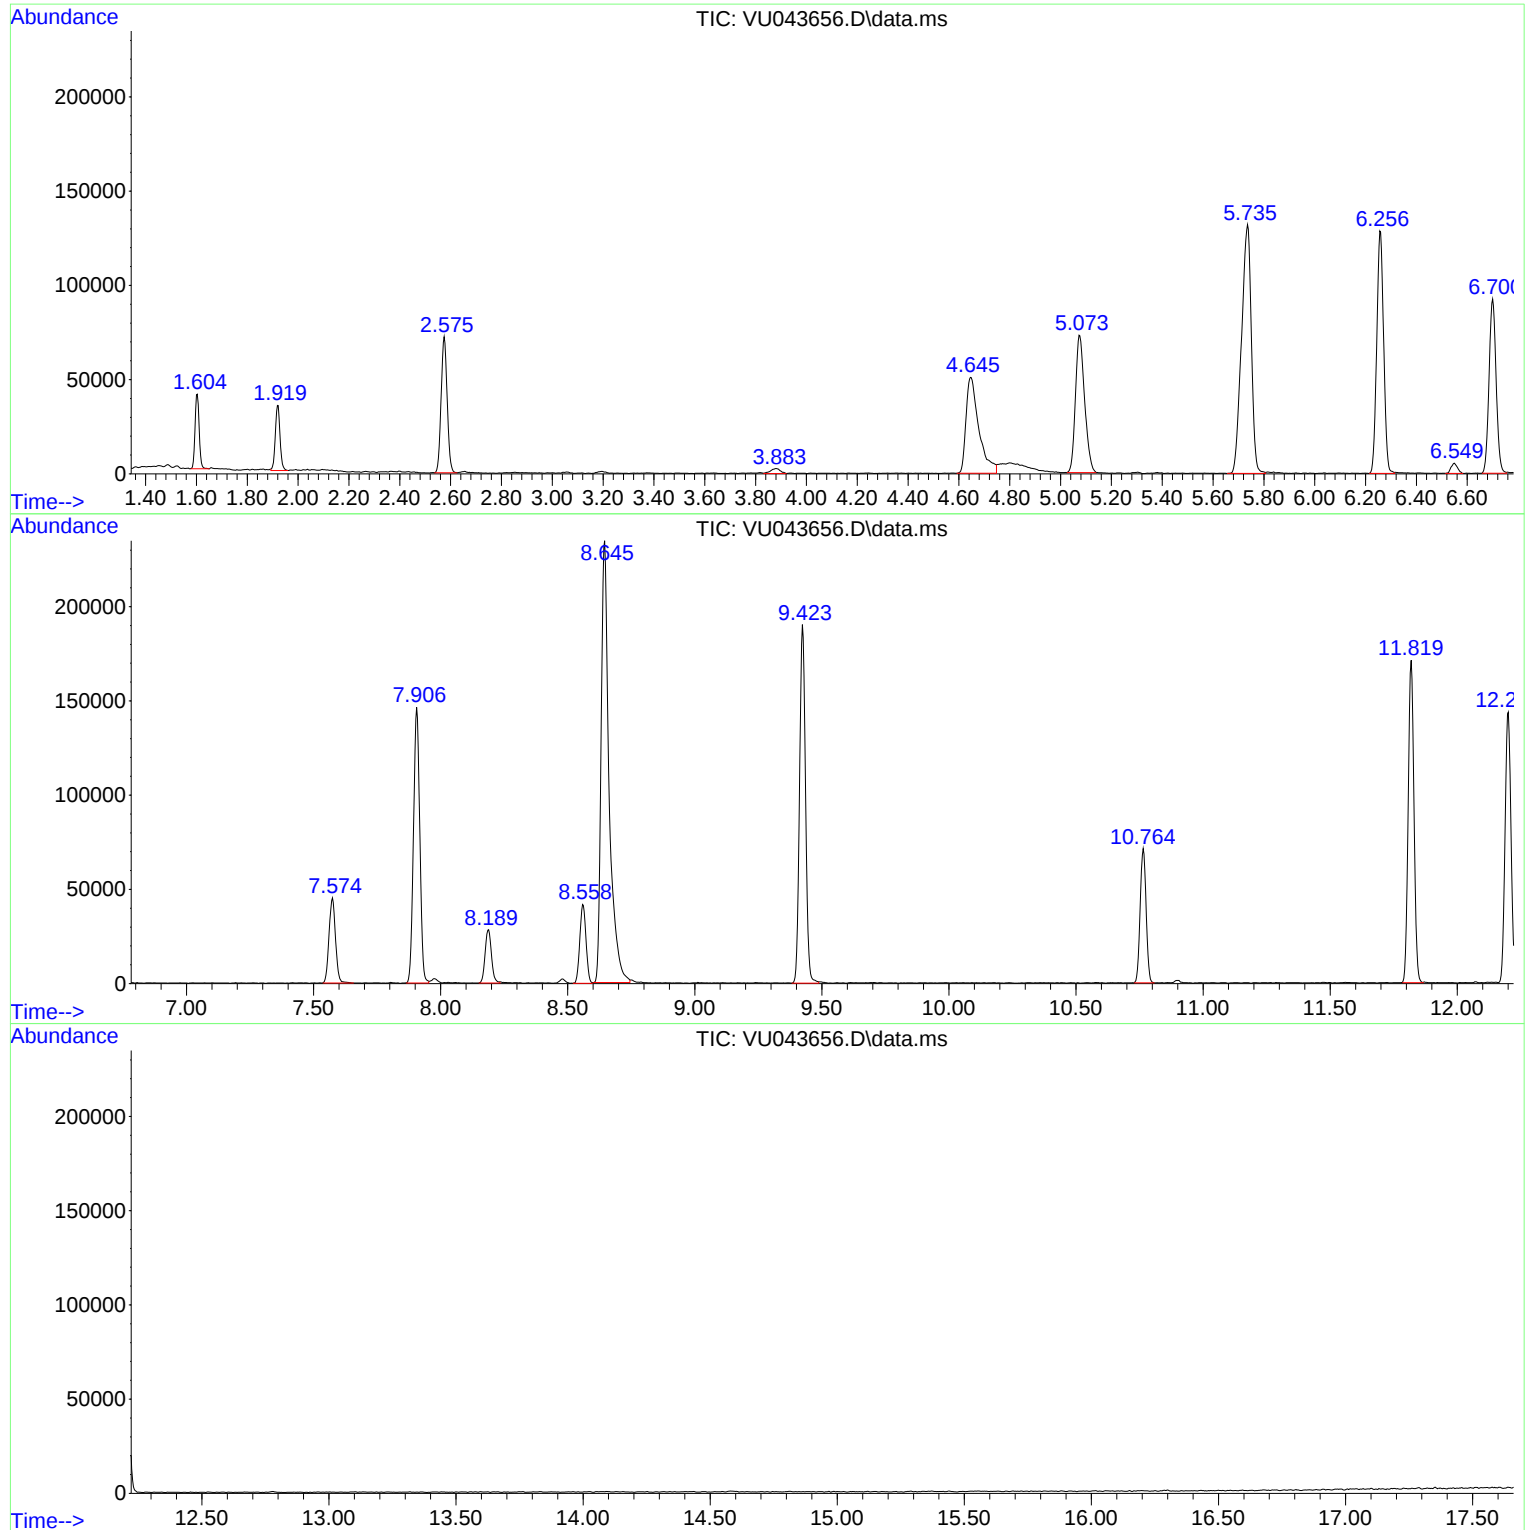

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU051121\  
Data File : VU043656.D  
Acq On : 11 May 2021 11:57  
Operator : SY/MD  
Sample : M2301-03  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BG6J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR050321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU051121\  
Data File : VU043656.D  
Acq On : 11 May 2021 11:57  
Operator : SY/MD  
Sample : M2301-03  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BG6J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR050321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----