

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051121\
 Data File : VU043660.D
 Acq On : 11 May 2021 13:32
 Operator : SY/MD
 Sample : M2320-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3A10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	52	rVV2	7736	8036	1.51%	0.248%
2	1.604	74	82	91	rBV	38077	42617	7.99%	1.316%
3	1.919	172	180	193	rVB	33631	43131	8.09%	1.331%
4	2.575	372	384	399	rBV	64371	105552	19.79%	3.258%
5	2.661	399	411	416	rBV3	3939	7733	1.45%	0.239%
6	4.652	1013	1030	1072	rBV	64217	230747	43.26%	7.123%
7	5.073	1146	1161	1182	rBV	73568	164524	30.85%	5.079%
8	5.735	1345	1367	1387	rBV3	136179	358624	67.24%	11.071%
9	6.256	1515	1529	1545	rBV	125882	235185	44.09%	7.260%
10	6.700	1654	1667	1686	rVB	93099	181764	34.08%	5.611%
11	7.574	1927	1939	1956	rVB3	45929	80525	15.10%	2.486%
12	7.906	2026	2042	2055	rBV	148516	252039	47.25%	7.780%
13	7.976	2056	2064	2075	rVB3	4245	7135	1.34%	0.220%
14	8.185	2118	2129	2141	rBV2	29627	48963	9.18%	1.511%
15	8.645	2259	2272	2302	rBV	279562	533379	100.00%	16.465%
16	9.423	2499	2514	2536	rBV	183205	300435	56.33%	9.274%
17	10.764	2919	2931	2945	rBV	75297	118871	22.29%	3.669%
18	11.819	3244	3259	3275	rBV	169144	263845	49.47%	8.145%
19	12.066	3328	3336	3350	rVB3	4711	7583	1.42%	0.234%
20	12.198	3365	3377	3398	rVB	148068	236339	44.31%	7.296%
21	12.896	3585	3594	3603	rVB4	8351	12408	2.33%	0.383%




Sum of corrected areas: 3239435

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051121\
Data File : VU043660.D
Acq On : 11 May 2021 13:32
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

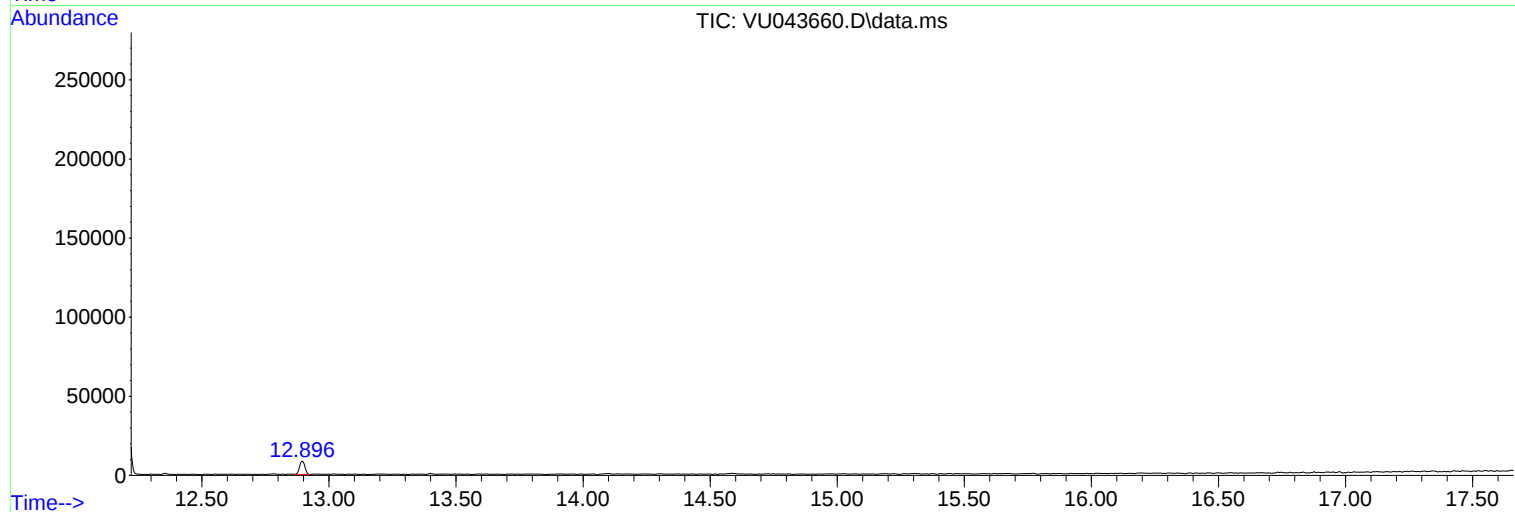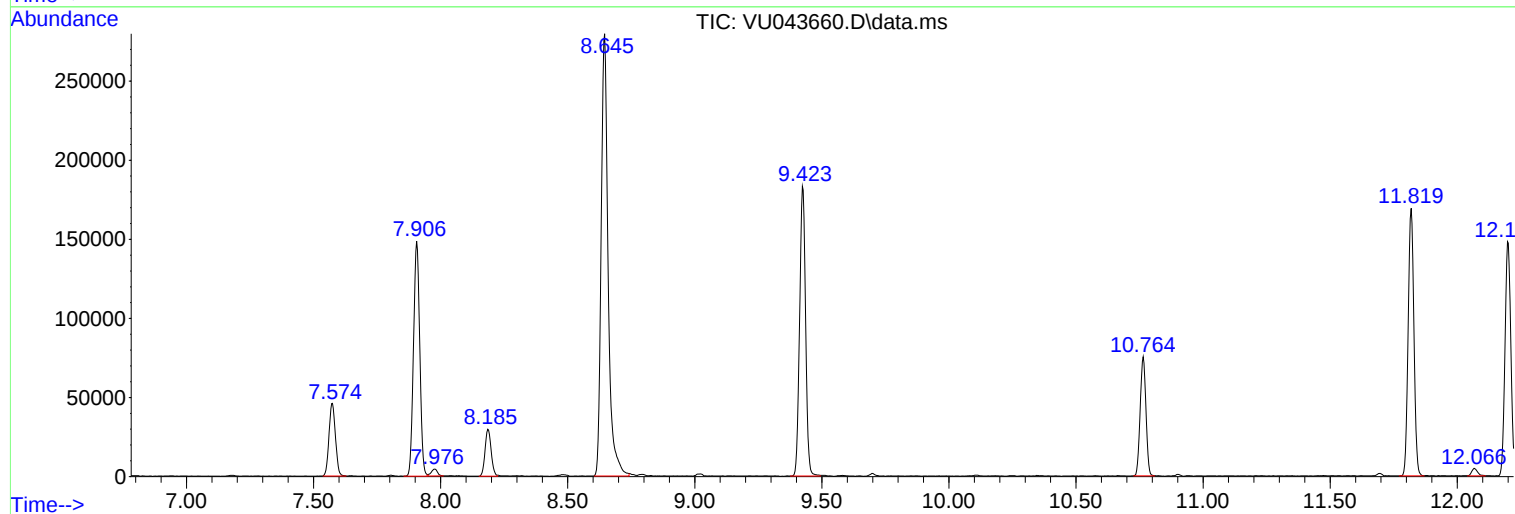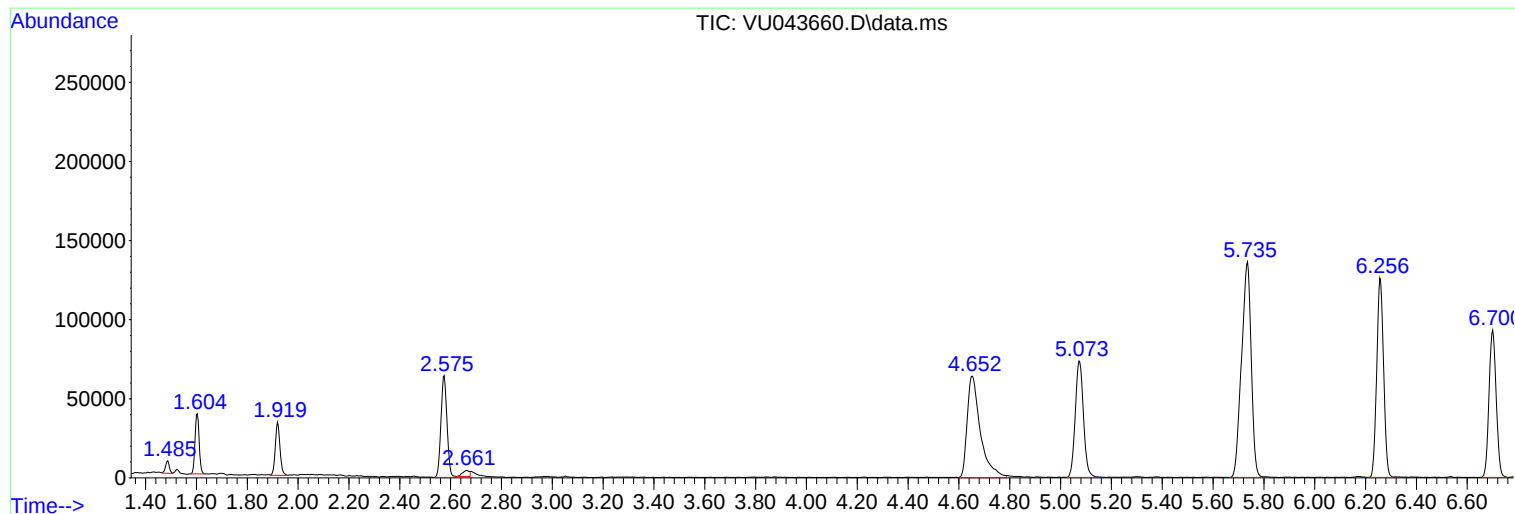

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051121\
Data File : VU043660.D
Acq On : 11 May 2021 13:32
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051121\
Data File : VU043660.D
Acq On : 11 May 2021 13:32
Operator : SY/MD
Sample : M2320-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3A10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
