

m/z	Abundance
36.00	1145.0
37.00	5850.0
38.00	5334.0
39.00	2162.0
40.10	206.0
43.90	1023.0
45.00	963.0
45.90	176.0
47.00	1258.0
47.90	716.0
49.00	4508.0
50.00	20136.0
51.00	6256.0
52.00	271.0
52.90	164.0
54.90	358.0
56.00	1452.0
57.00	2704.0
57.80	154.0
60.00	954.0
61.00	5190.0
62.00	4891.0
63.00	4114.0
64.00	614.0
65.00	904.0
66.90	262.0
68.00	9512.0
69.00	9416.0
69.90	799.0
71.90	481.0
73.00	4176.0
74.00	16070.0
75.00	45944.0
76.00	3924.0
76.90	534.0
77.80	304.0
78.90	4014.0
79.90	1141.0
80.90	4006.0
81.90	1026.0
82.90	108.0
85.90	110.0
86.90	2918.0
87.90	3037.0
90.90	368.0
92.00	2556.0
92.90	4069.0
94.00	10885.0
95.00	79832.0
96.00	5085.0
97.00	211.0
103.80	437.0
104.80	138.0
105.80	448.0
111.80	103.0
112.90	111.0
115.80	389.0
116.90	809.0
117.80	382.0
118.90	574.0
127.90	268.0
128.90	152.0
129.80	321.0
134.70	110.0
136.90	138.0
140.90	855.0
142.00	168.0
142.80	1256.0
144.80	363.0
145.90	136.0
147.80	219.0
154.80	180.0
170.80	195.0
171.90	980.0
173.90	60456.0
174.90	5054.0
175.90	59240.0
176.90	4149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
39.80	119.0
43.90	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
36.00	984.0
37.00	5308.0
38.00	4373.0
39.00	1788.0
40.10	233.0
44.00	828.0
45.00	863.0
45.90	135.0
47.00	1058.0
48.00	554.0
49.00	4022.0
50.00	18968.0
51.00	5715.0
52.00	219.0
52.90	131.0
54.90	242.0
56.00	1376.0
57.00	2474.0
59.90	862.0
61.00	4697.0
62.00	4722.0
63.00	3811.0
63.90	451.0
65.00	814.0
67.00	270.0
68.00	8610.0
69.00	8626.0
70.00	697.0
71.90	414.0
73.00	3894.0
74.00	15035.0
75.00	42216.0
76.00	3445.0
76.90	486.0
77.90	266.0
78.90	3471.0
79.90	1055.0
80.90	3566.0
81.90	819.0
82.80	104.0
85.90	119.0
86.90	2505.0
87.90	2656.0
90.80	367.0
91.90	2487.0
93.00	3700.0
94.00	9802.0
95.00	74528.0
96.00	4815.0
97.00	171.0
103.90	383.0
104.90	116.0
105.80	363.0
115.80	330.0
116.90	787.0
117.80	332.0
118.90	490.0
127.80	264.0
128.80	171.0
129.90	258.0
130.80	142.0
134.70	109.0
136.80	136.0
140.90	897.0
142.80	1056.0
144.80	282.0
145.80	103.0
147.80	268.0
154.90	172.0
170.90	157.0
171.90	1147.0
173.00	1224.0
173.90	60304.0
174.90	5002.0
175.90	57904.0
176.90	3824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB142

m/z	Abundance
36.00	1115.0
37.00	5851.0
38.00	5002.0
39.00	2000.0
40.10	236.0
43.90	909.0
45.00	1002.0
45.90	174.0
47.00	1214.0
48.00	690.0
49.00	4529.0
50.00	20776.0
51.00	6271.0
52.00	280.0
52.90	160.0
54.90	300.0
56.00	1446.0
57.00	2719.0
57.90	124.0
59.90	919.0
61.00	5189.0
62.00	5065.0
63.00	4103.0
63.90	533.0
65.00	908.0
66.90	278.0
68.00	9502.0
69.00	9355.0
70.00	775.0
71.90	476.0
73.00	4293.0
74.00	16244.0
75.00	46168.0
76.00	3865.0
76.90	564.0
77.90	299.0
78.90	3897.0
79.90	1141.0
80.90	3965.0
81.90	943.0
82.80	118.0
85.90	126.0
86.90	2660.0
87.90	2909.0
90.90	393.0
91.90	2698.0
93.00	4089.0
94.00	10795.0
95.00	81144.0
96.00	5292.0
97.00	193.0
103.90	410.0
104.80	126.0
105.80	420.0
113.00	116.0
115.80	380.0
116.90	876.0
117.80	396.0
118.90	552.0
127.80	283.0
128.80	169.0
129.90	299.0
130.80	129.0
134.70	119.0
136.80	141.0
140.90	936.0
142.00	137.0
142.80	1206.0
144.80	344.0
145.90	131.0
147.80	257.0
149.80	104.0
154.90	209.0
170.80	186.0
171.90	1140.0
173.90	63600.0
174.90	5272.0
175.90	61448.0
176.90	4217.0



Instrument :
MSVOA_U
ClientSampleId :
BFB142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051121\
 Data File : VU043652.D
 Acq On : 11 May 2021 09:32
 Operator : SY/MD
 Sample : BFB42
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB142

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 12 01:26:46 2021

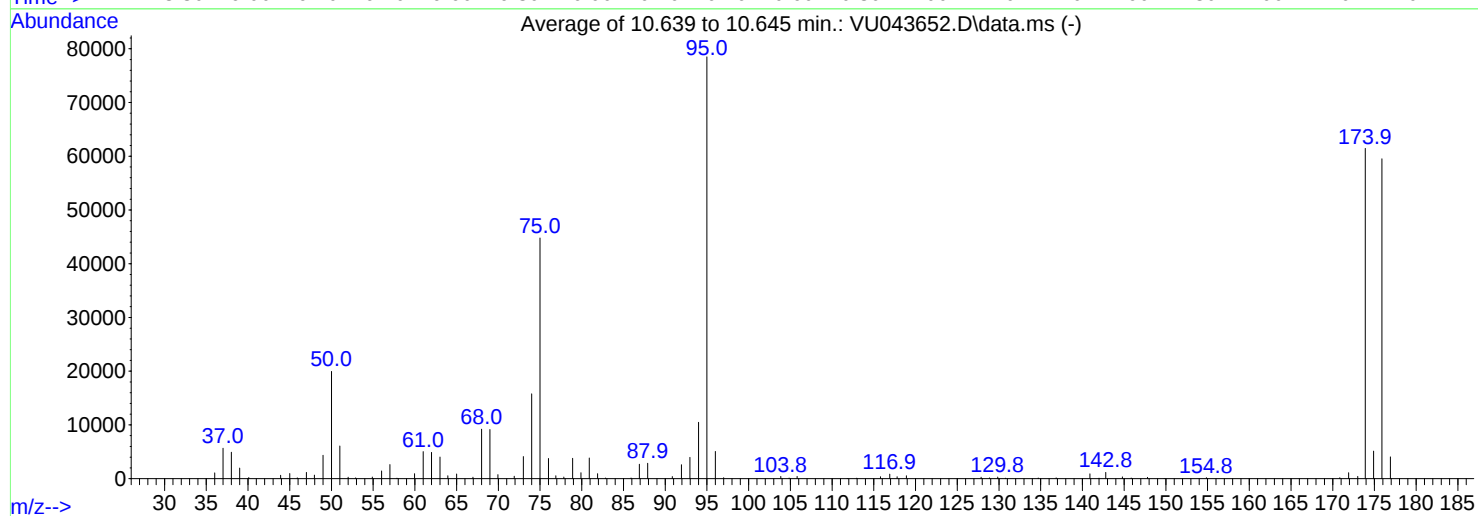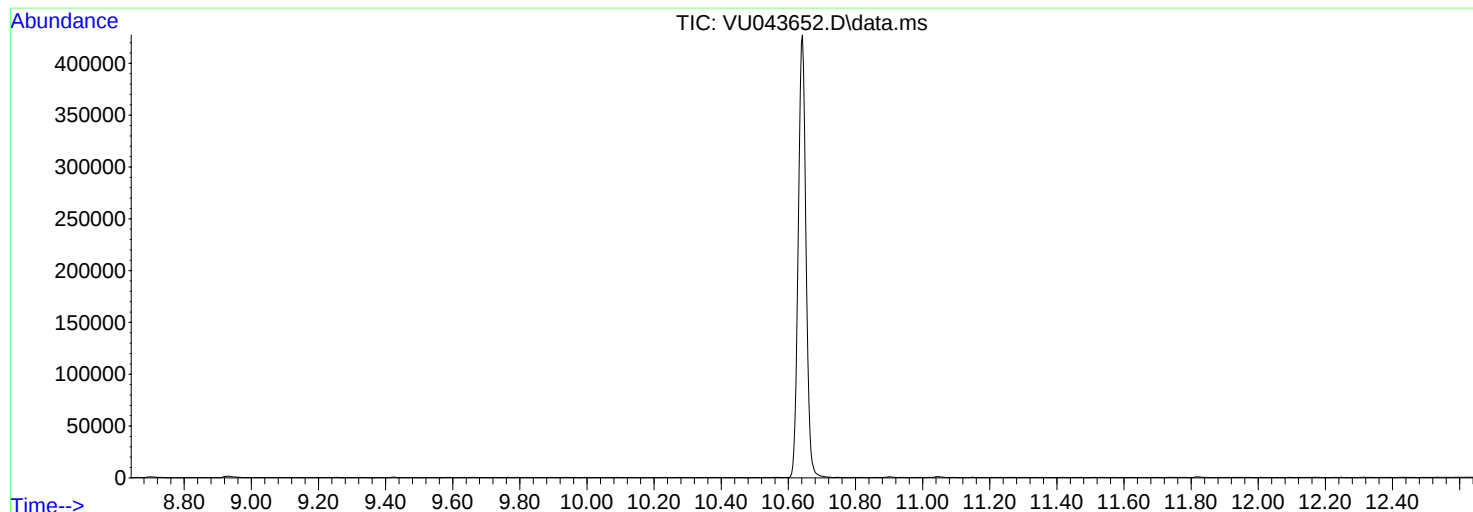

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	19960	PASS
75	95	30	80	57.0	44776	PASS
95	95	100	100	100.0	78501	PASS
96	95	5	9	6.5	5064	PASS
173	174	0.00	2	0.7	408	PASS
174	95	50	120	78.3	61453	PASS
175	174	5	9	8.3	5109	PASS
176	174	95	101	96.9	59531	PASS
177	176	5	9	6.8	4063	PASS