

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048511.D
 Acq On : 11 May 2022 12:43
 Operator : SY/MD
 Sample : N2736-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX1

Quant Time: May 12 03:42:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	267901	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	265302	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	139330	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	60116	26.056	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	52.120%#		
7) Chloroethane-d5	1.912	69	53295	35.394	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	70.780%		
11) 1,1-Dichloroethene-d2	2.568	63	110846	26.995	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	53.980%#		
21) 2-Butanone-d5	4.620	46	160051	81.455	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.450%		
24) Chloroform-d	5.063	84	177440	44.277	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.560%		
26) 1,2-Dichloroethane-d4	5.703	65	130578	50.126	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.260%		
32) Benzene-d6	5.729	84	323879	40.174	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.340%		
36) 1,2-Dichloropropane-d6	6.690	67	101540	38.623	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	77.240%		
41) Toluene-d8	7.899	98	283857	39.811	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.620%#		
43) trans-1,3-Dichloroprop...	8.182	79	56592	46.769	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.540%		
47) 2-Hexanone-d5	8.632	63	115027	90.398	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.400%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	161257	40.268	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.540%		
66) 1,2-Dichlorobenzene-d4	12.192	152	129174	46.820	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.640%		
Target Compounds					Qvalue	
13) Acetone	2.626	43	17068	11.522	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048511.D
Acq On : 11 May 2022 12:43
Operator : SY/MD
Sample : N2736-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEX1

Quant Time: May 12 03:42:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

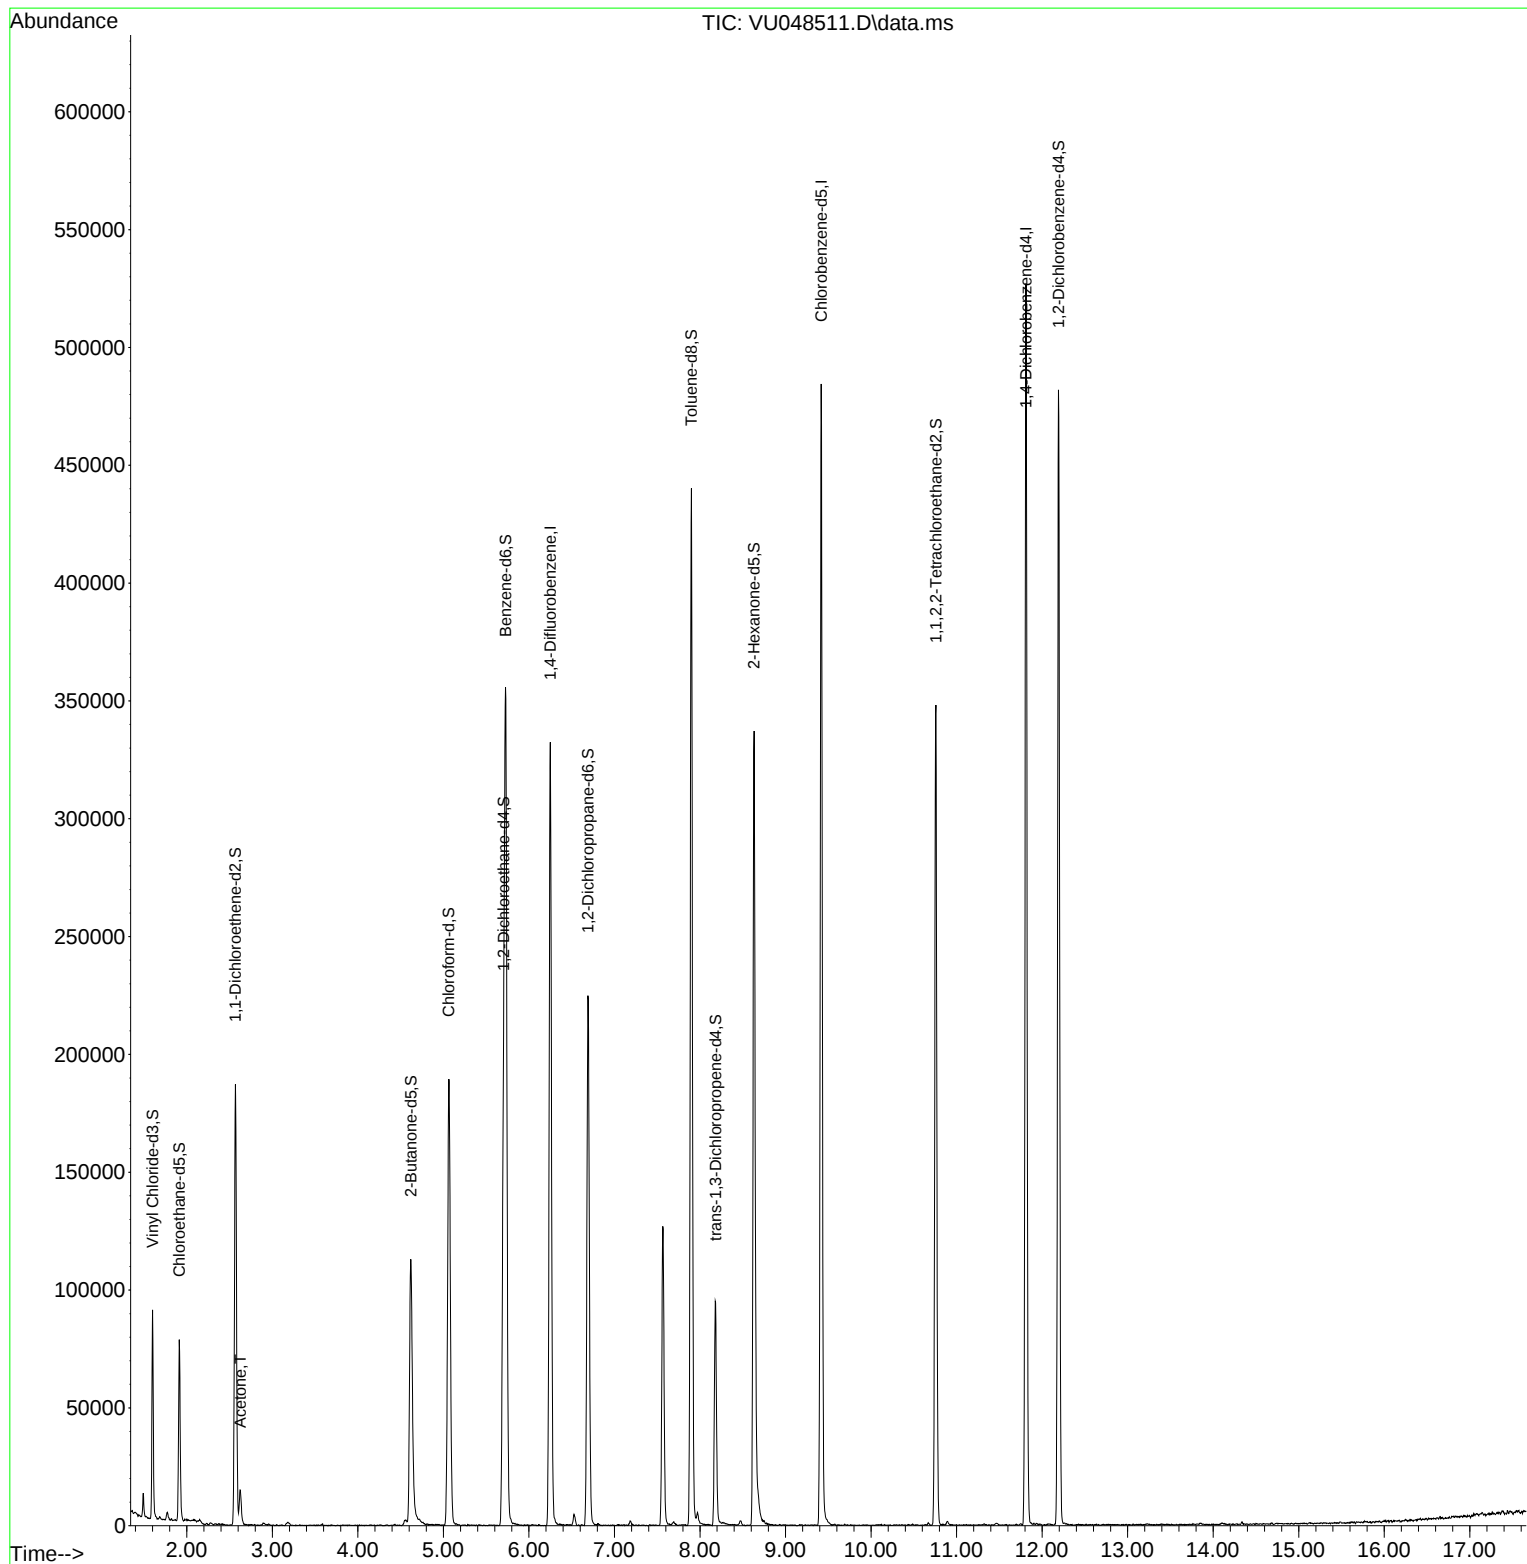

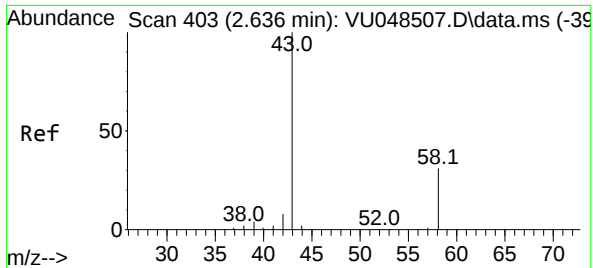

#13
 Acetone
 Concen: 11.522 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.010 min
 Lab File: VU048511.D
 Acq: 11 May 2022 12:43

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX1

Tgt Ion: 43 Resp: 17068
 Ion Ratio Lower Upper
 43 100
 58 29.6 0.0 66.2

