

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048516.D
 Acq On : 11 May 2022 14:55
 Operator : SY/MD
 Sample : N2790-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNI

Quant Time: May 12 03:43:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	273593	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	279582	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	145559	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	84978	36.065	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.140%
7) Chloroethane-d5	1.912	69	64631	42.029	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.060%
11) 1,1-Dichloroethene-d2	2.568	63	136345	32.514	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.020%
21) 2-Butanone-d5	4.623	46	158862	79.167	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.170%
24) Chloroform-d	5.066	84	197881	48.351	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.700%
26) 1,2-Dichloroethane-d4	5.703	65	142810	53.681	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.360%
32) Benzene-d6	5.729	84	370909	43.657	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.320%
36) 1,2-Dichloropropane-d6	6.690	67	111897	40.389	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.780%
41) Toluene-d8	7.899	98	338472	45.046	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.100%
43) trans-1,3-Dichloroprop...	8.179	79	61256	48.038	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.080%
47) 2-Hexanone-d5	8.632	63	121260	90.429	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.430%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	171175	40.562	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.120%
66) 1,2-Dichlorobenzene-d4	12.192	152	142115	49.306	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.620%
Target Compounds						
					Qvalue	
13) Acetone	2.633	43	6045	3.996	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048516.D
Acq On : 11 May 2022 14:55
Operator : SY/MD
Sample : N2790-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN1

Quant Time: May 12 03:43:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

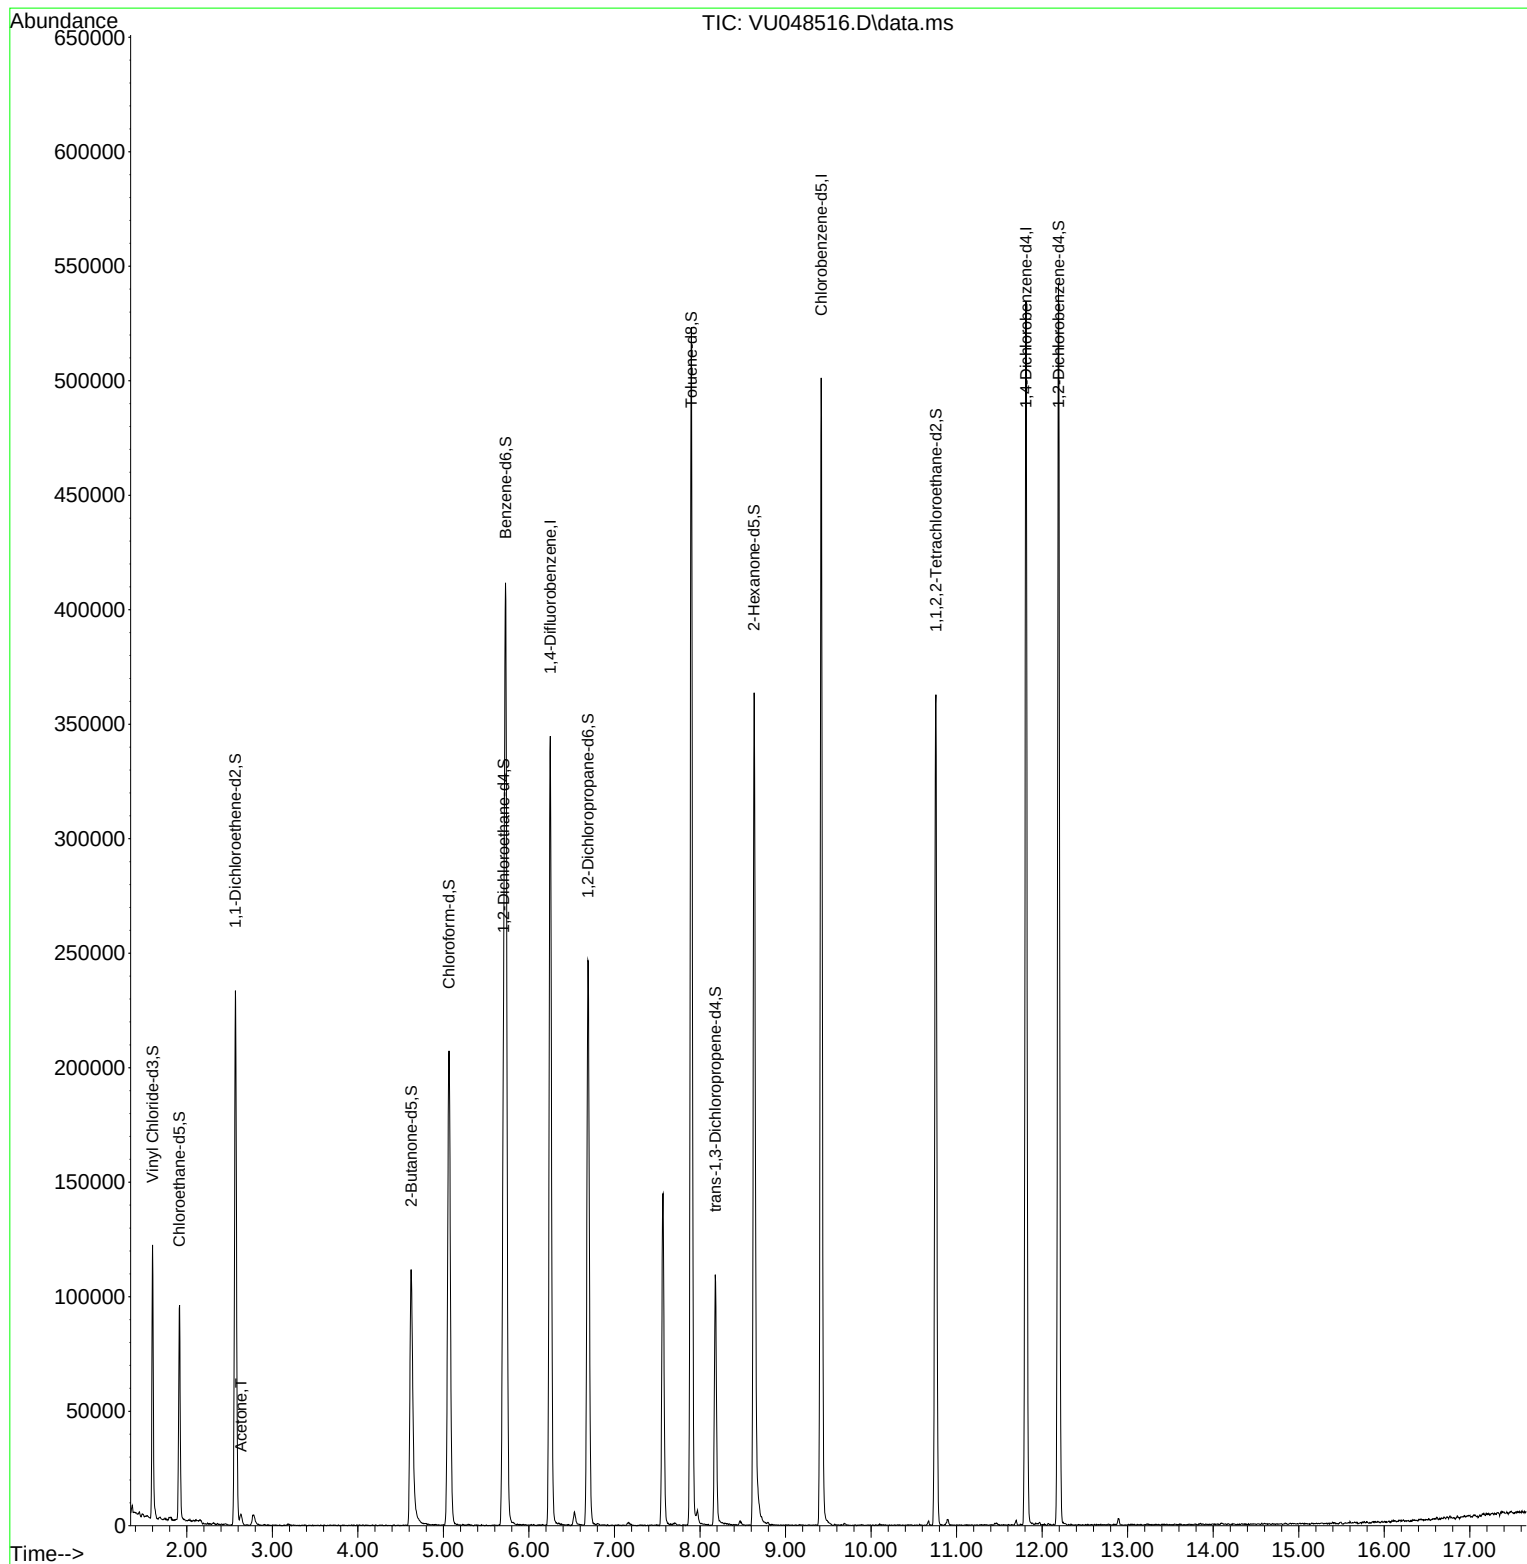

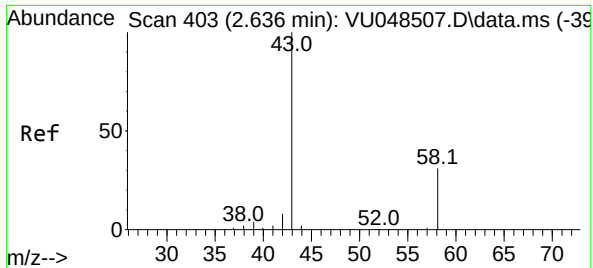

#13
 Acetone
 Concen: 3.996 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU048516.D
 Acq: 11 May 2022 14:55

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPN1

Tgt Ion: 43 Resp: 6045
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 66.2

