

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048517.D
 Acq On : 11 May 2022 15:19
 Operator : SY/MD
 Sample : N2790-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP2

Quant Time: May 12 03:43:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	259291	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	258501	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	135262	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	84349	37.773	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.540%
7) Chloroethane-d5	1.913	69	65755	45.119	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.240%
11) 1,1-Dichloroethene-d2	2.568	63	137962	34.714	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.420%
21) 2-Butanone-d5	4.623	46	164955	86.738	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.740%
24) Chloroform-d	5.064	84	195765	50.472	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.940%
26) 1,2-Dichloroethane-d4	5.703	65	145490	57.705	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.400%
32) Benzene-d6	5.729	84	371429	47.284	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.560%
36) 1,2-Dichloropropane-d6	6.690	67	112863	44.060	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.120%
41) Toluene-d8	7.899	98	336511	48.437	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.880%
43) trans-1,3-Dichloroprop...	8.179	79	62529	53.035	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	106.060%
47) 2-Hexanone-d5	8.632	63	123420	99.546	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.550%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	170832	43.782	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.560%
66) 1,2-Dichlorobenzene-d4	12.192	152	140642	52.510	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.020%
Target Compounds						
13) Acetone	2.633	43	5617	3.918	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048517.D
Acq On : 11 May 2022 15:19
Operator : SY/MD
Sample : N2790-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN2

Quant Time: May 12 03:43:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

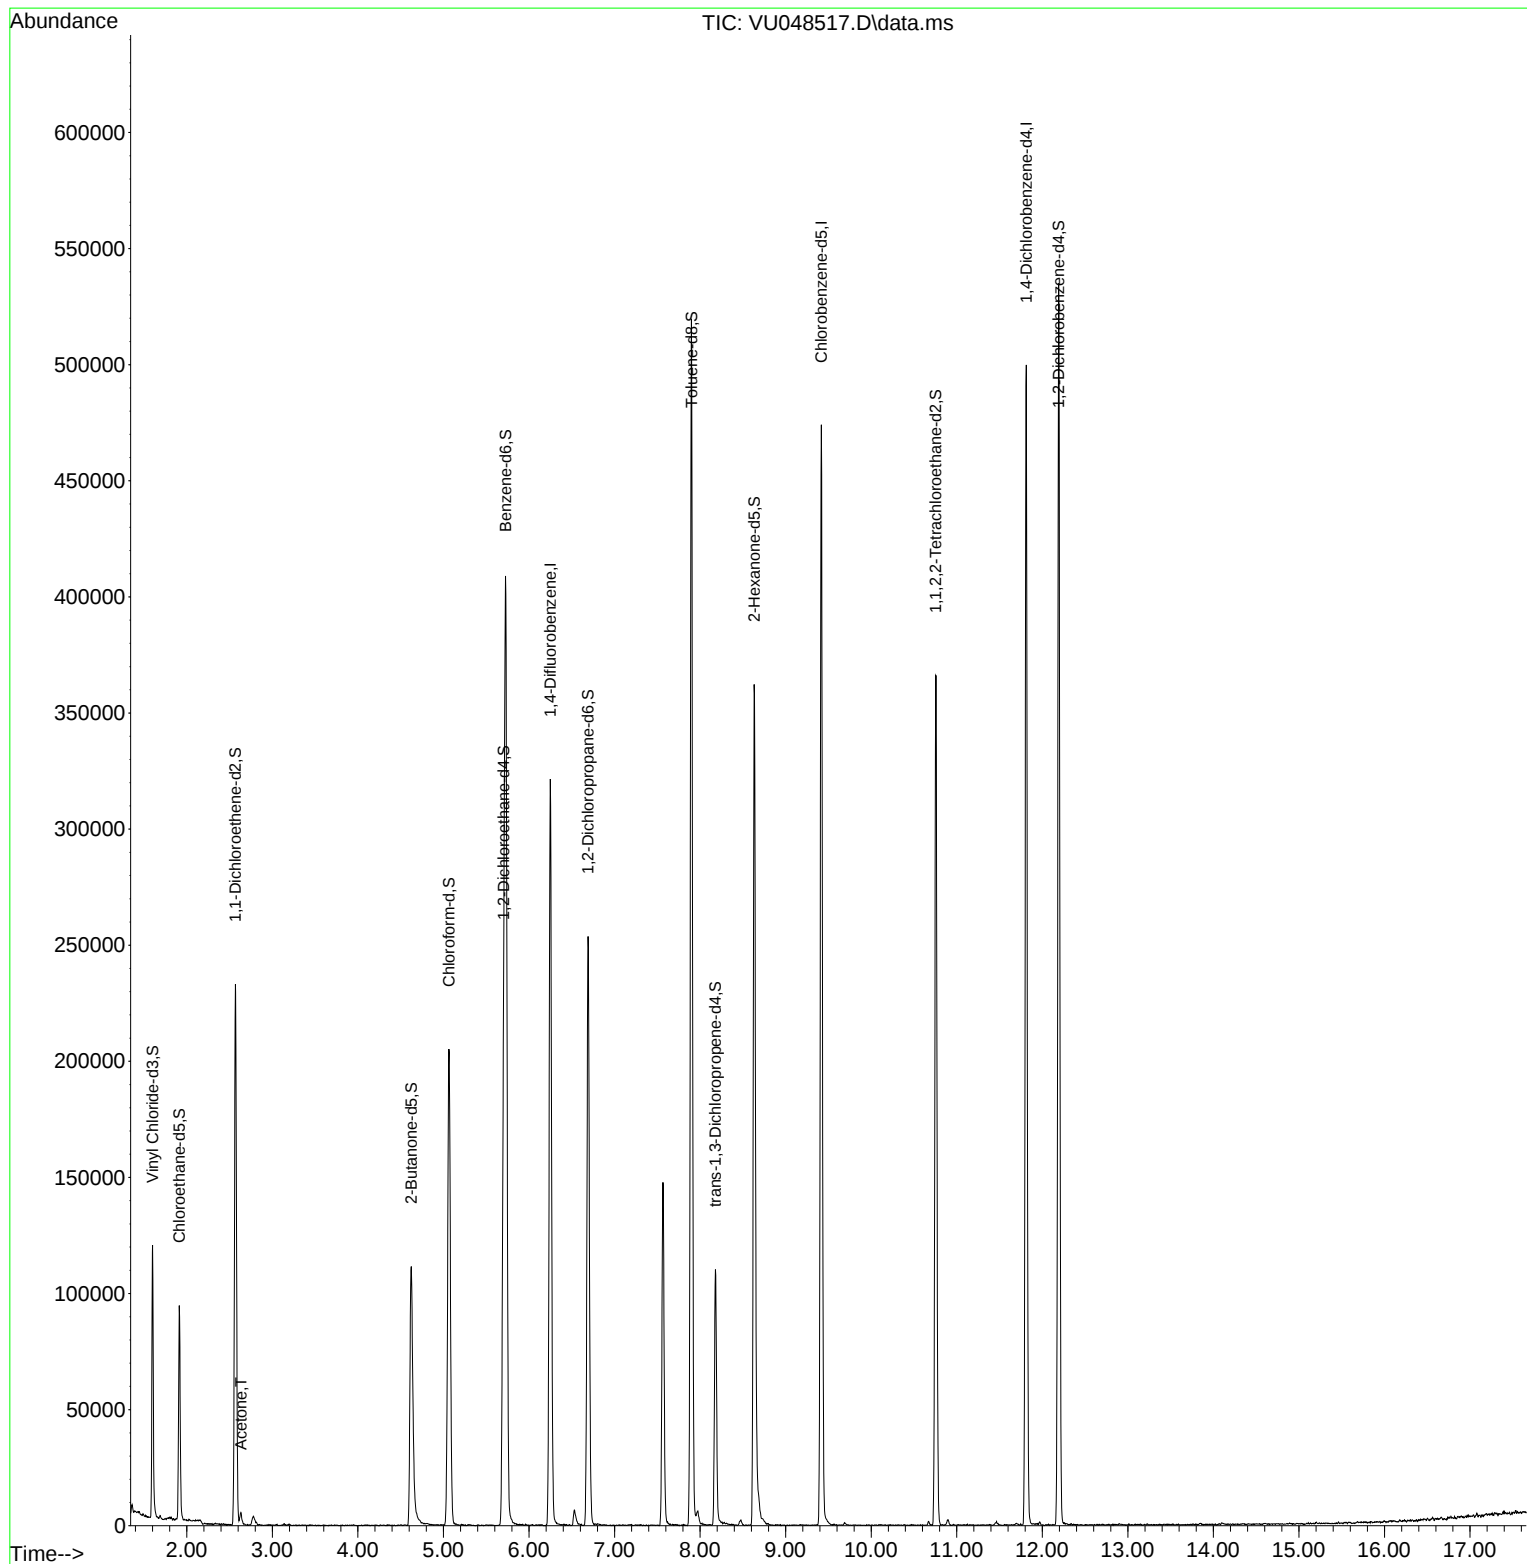

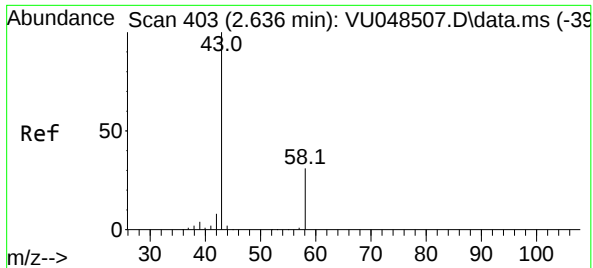

#13
 Acetone
 Concen: 3.918 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU048517.D
 Acq: 11 May 2022 15:19

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP2

Tgt Ion: 43 Resp: 5617
 Ion Ratio Lower Upper
 43 100
 58 26.0 0.0 66.2

