

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048521.D
 Acq On : 11 May 2022 16:52
 Operator : SY/MD
 Sample : N2790-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP6

Quant Time: May 12 03:44:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	262548	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	264649	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	139353	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	80708	35.694	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.380%
7) Chloroethane-d5	1.912	69	63122	42.775	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.540%
11) 1,1-Dichloroethene-d2	2.568	63	128910	32.034	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.060%
21) 2-Butanone-d5	4.623	46	152232	79.055	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.050%
24) Chloroform-d	5.067	84	189851	48.340	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.680%
26) 1,2-Dichloroethane-d4	5.703	65	139927	54.810	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.620%
32) Benzene-d6	5.729	84	356795	44.366	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.740%
36) 1,2-Dichloropropane-d6	6.690	67	107843	41.122	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.240%
41) Toluene-d8	7.899	98	322710	45.372	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.740%
43) trans-1,3-Dichloroprop...	8.179	79	59731	49.485	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.960%
47) 2-Hexanone-d5	8.632	63	112900	88.945	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.950%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	167094	41.829	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.660%
66) 1,2-Dichlorobenzene-d4	12.192	152	137659	49.887	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.780%
Target Compounds						
13) Acetone	2.629	43	18770	12.929	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048521.D
Acq On : 11 May 2022 16:52
Operator : SY/MD
Sample : N2790-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN6


Quant Time: May 12 03:44:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

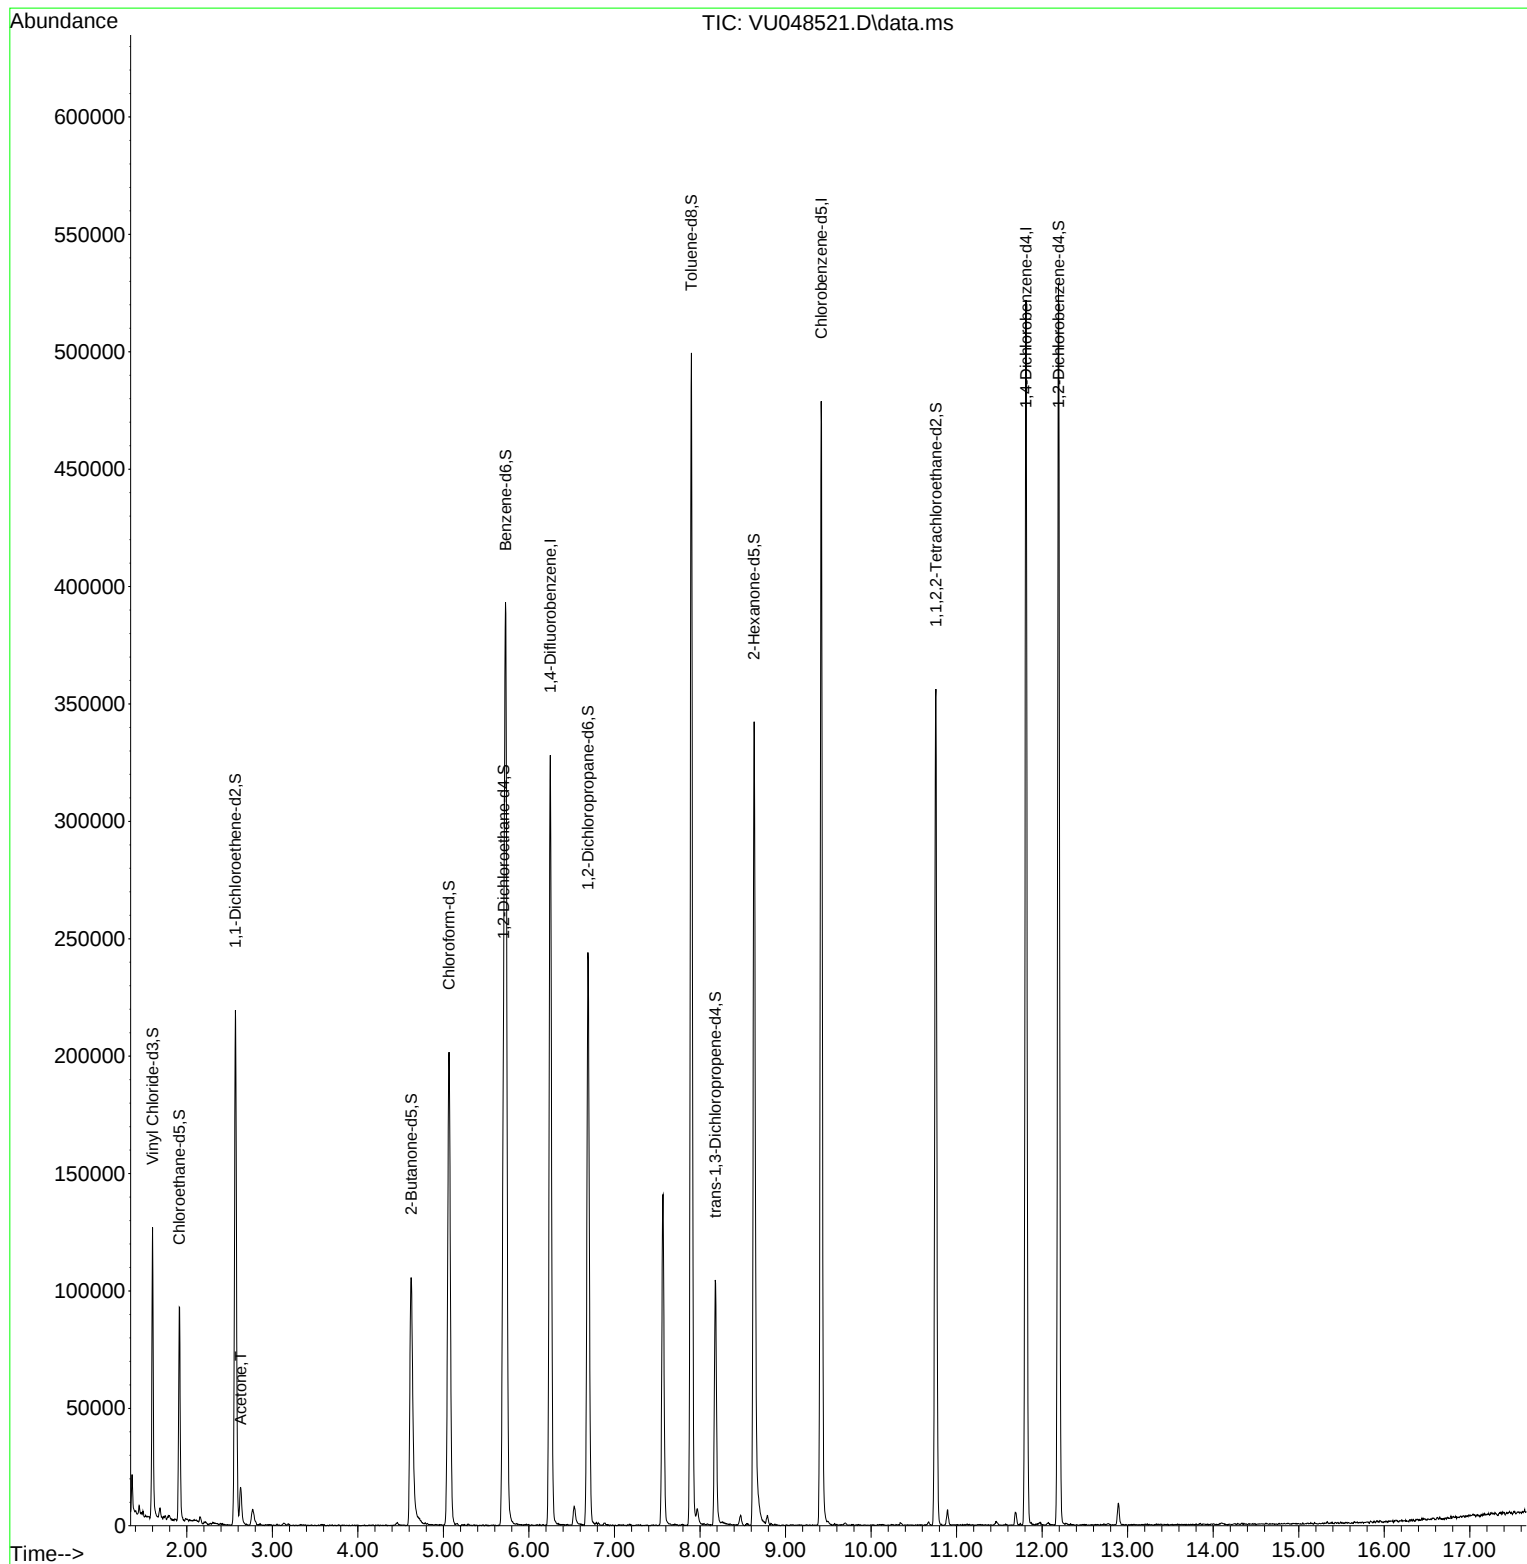

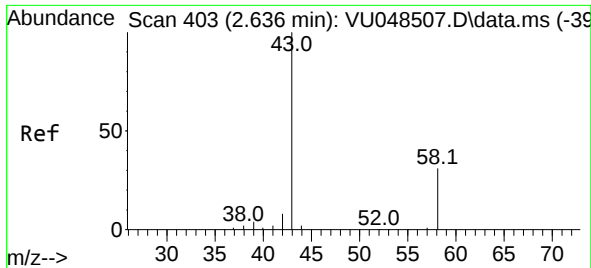

#13
 Acetone
 Concen: 12.929 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. -0.006 min
 Lab File: VU048521.D
 Acq: 11 May 2022 16:52

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP6

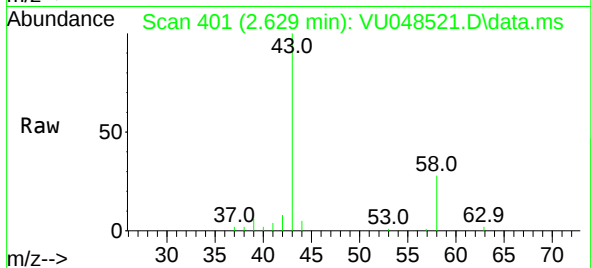

Tgt Ion: 43 Resp: 18770
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 66.2

