

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048525.D
 Acq On : 11 May 2022 18:25
 Operator : SY/MD
 Sample : N2790-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNO

Quant Time: May 12 03:45:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	280720	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	278732	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	143898	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	79443	32.860	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.720%
7) Chloroethane-d5	1.912	69	61180	38.775	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	77.540%
11) 1,1-Dichloroethene-d2	2.568	63	130122	30.242	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.480%
21) 2-Butanone-d5	4.620	46	159375	77.407	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	77.410%
24) Chloroform-d	5.067	84	195648	46.591	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.180%
26) 1,2-Dichloroethane-d4	5.703	65	139255	51.015	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.040%
32) Benzene-d6	5.729	84	358441	42.318	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.640%
36) 1,2-Dichloropropane-d6	6.690	67	111807	40.479	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.960%
41) Toluene-d8	7.899	98	329266	43.954	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.900%
43) trans-1,3-Dichloroprop...	8.179	79	59586	46.870	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.740%
47) 2-Hexanone-d5	8.632	63	117959	88.235	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.240%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	167761	39.874	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.740%
66) 1,2-Dichlorobenzene-d4	12.195	152	139930	49.109	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.220%
Target Compounds						
13) Acetone	2.633	43	3832	2.469	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048525.D
Acq On : 11 May 2022 18:25
Operator : SY/MD
Sample : N2790-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPNO


Quant Time: May 12 03:45:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

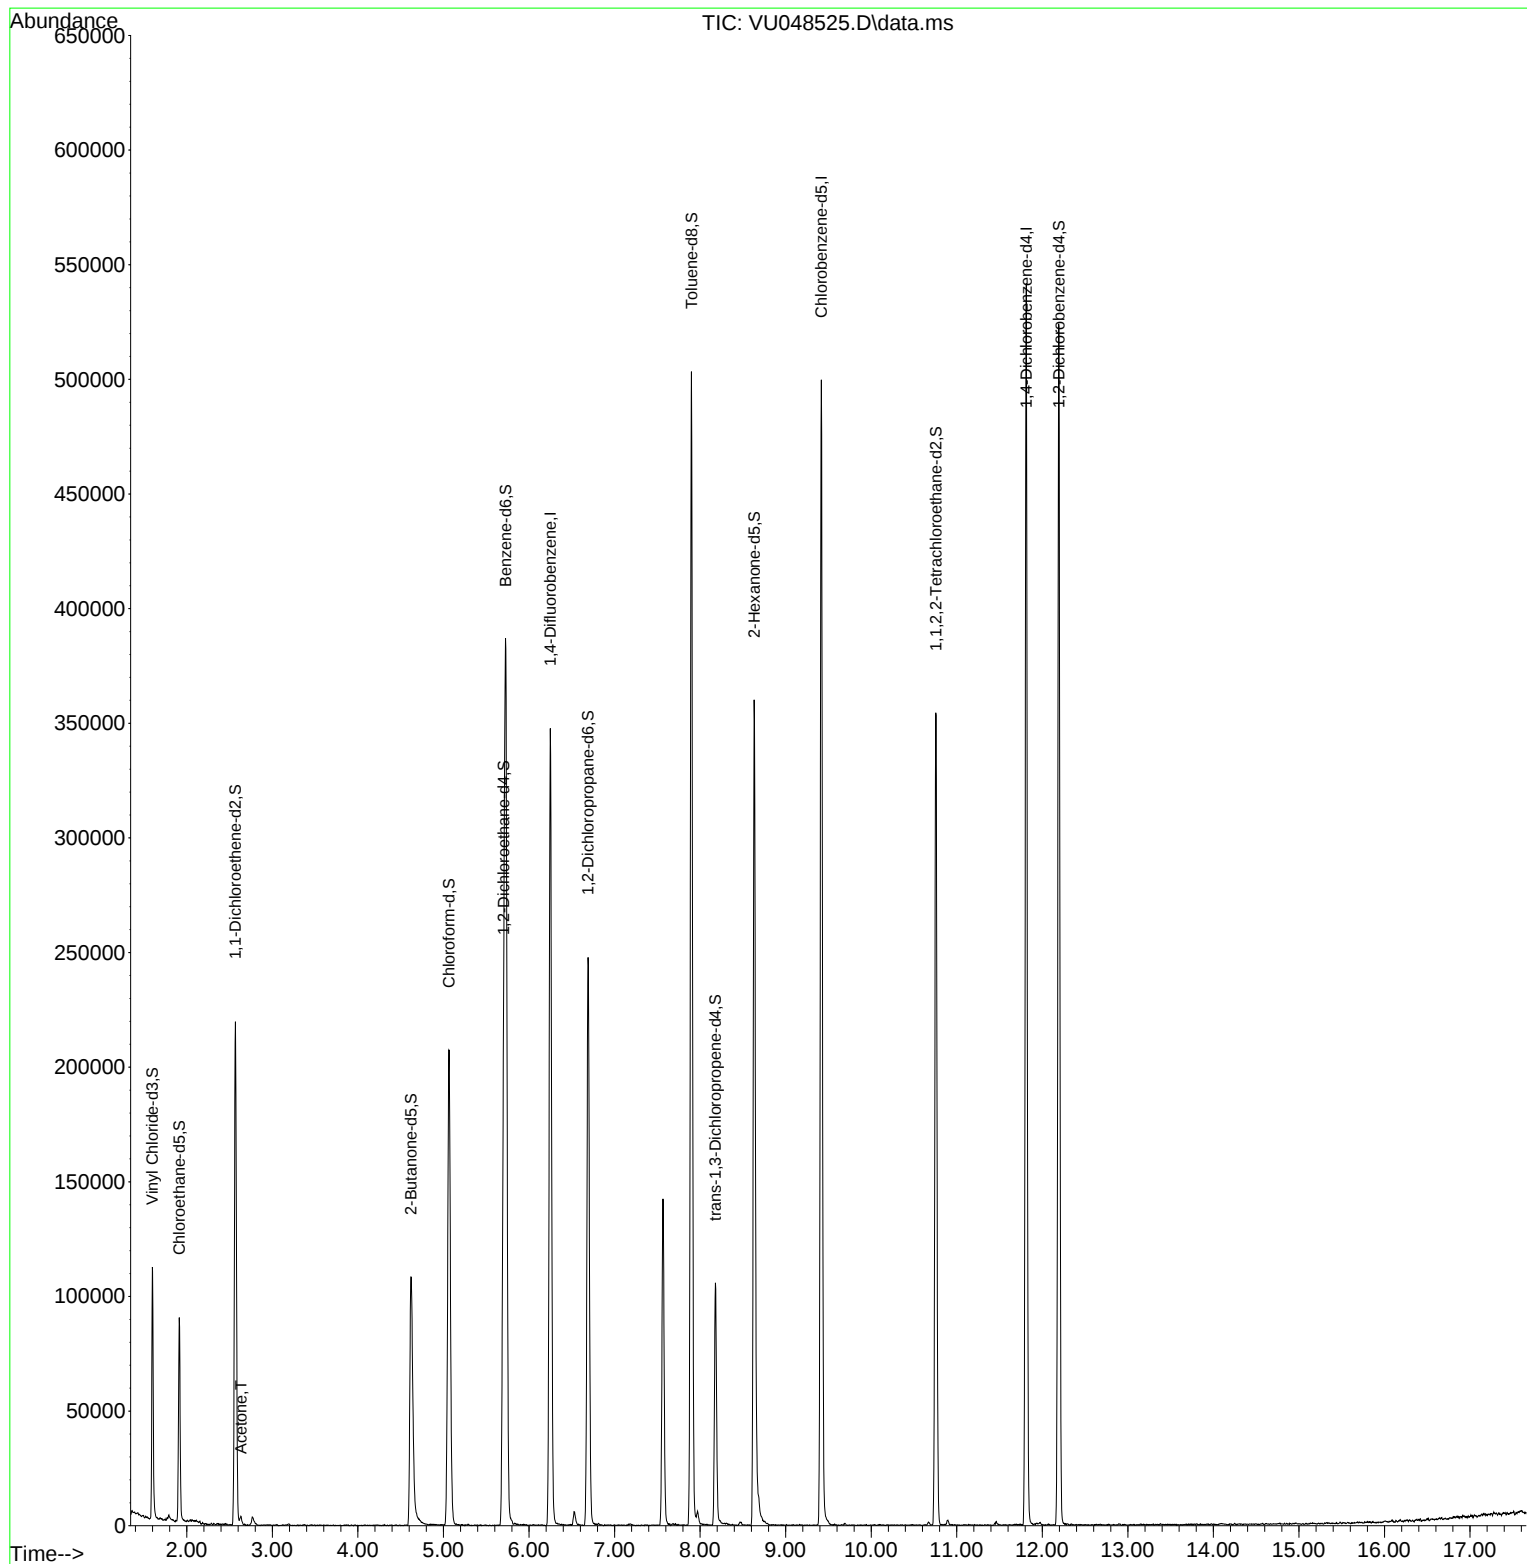

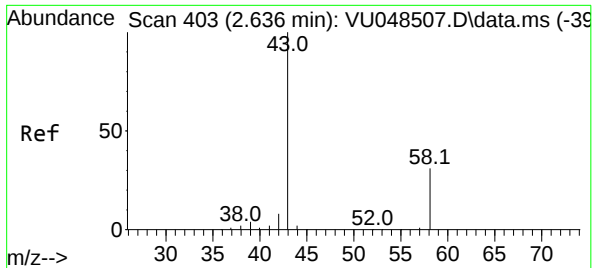

#13
 Acetone
 Concen: 2.469 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU048525.D
 Acq: 11 May 2022 18:25

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNO

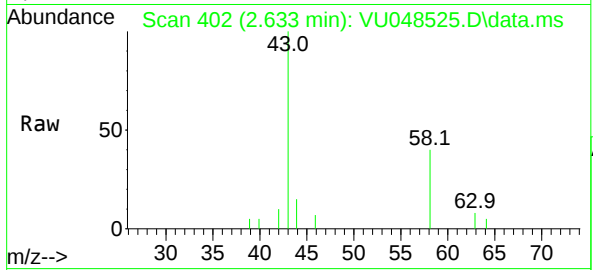

Tgt Ion: 43 Resp: 3832
 Ion Ratio Lower Upper
 43 100
 58 33.5 0.0 66.2

