

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048526.D
 Acq On : 11 May 2022 18:48
 Operator : SY/MD
 Sample : N2790-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP9

Quant Time: May 12 03:45:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	279114	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	277228	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	144745	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	84364	35.096	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.200%
7) Chloroethane-d5	1.912	69	64450	41.082	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.160%
11) 1,1-Dichloroethene-d2	2.568	63	135091	31.578	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.160%
21) 2-Butanone-d5	4.616	46	164422	80.317	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.320%
24) Chloroform-d	5.063	84	199792	47.852	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.700%
26) 1,2-Dichloroethane-d4	5.703	65	142972	52.678	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.360%
32) Benzene-d6	5.729	84	372005	44.158	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.320%
36) 1,2-Dichloropropane-d6	6.690	67	113443	41.294	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.580%
41) Toluene-d8	7.899	98	337667	45.320	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.640%
43) trans-1,3-Dichloroprop...	8.179	79	60379	47.752	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.500%
47) 2-Hexanone-d5	8.629	63	119000	89.497	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.500%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	174294	41.652	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.300%
66) 1,2-Dichlorobenzene-d4	12.192	152	144743	50.500	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						
					Qvalue	
13) Acetone	2.623	43	5205	3.372	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048526.D
Acq On : 11 May 2022 18:48
Operator : SY/MD
Sample : N2790-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP9

Quant Time: May 12 03:45:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

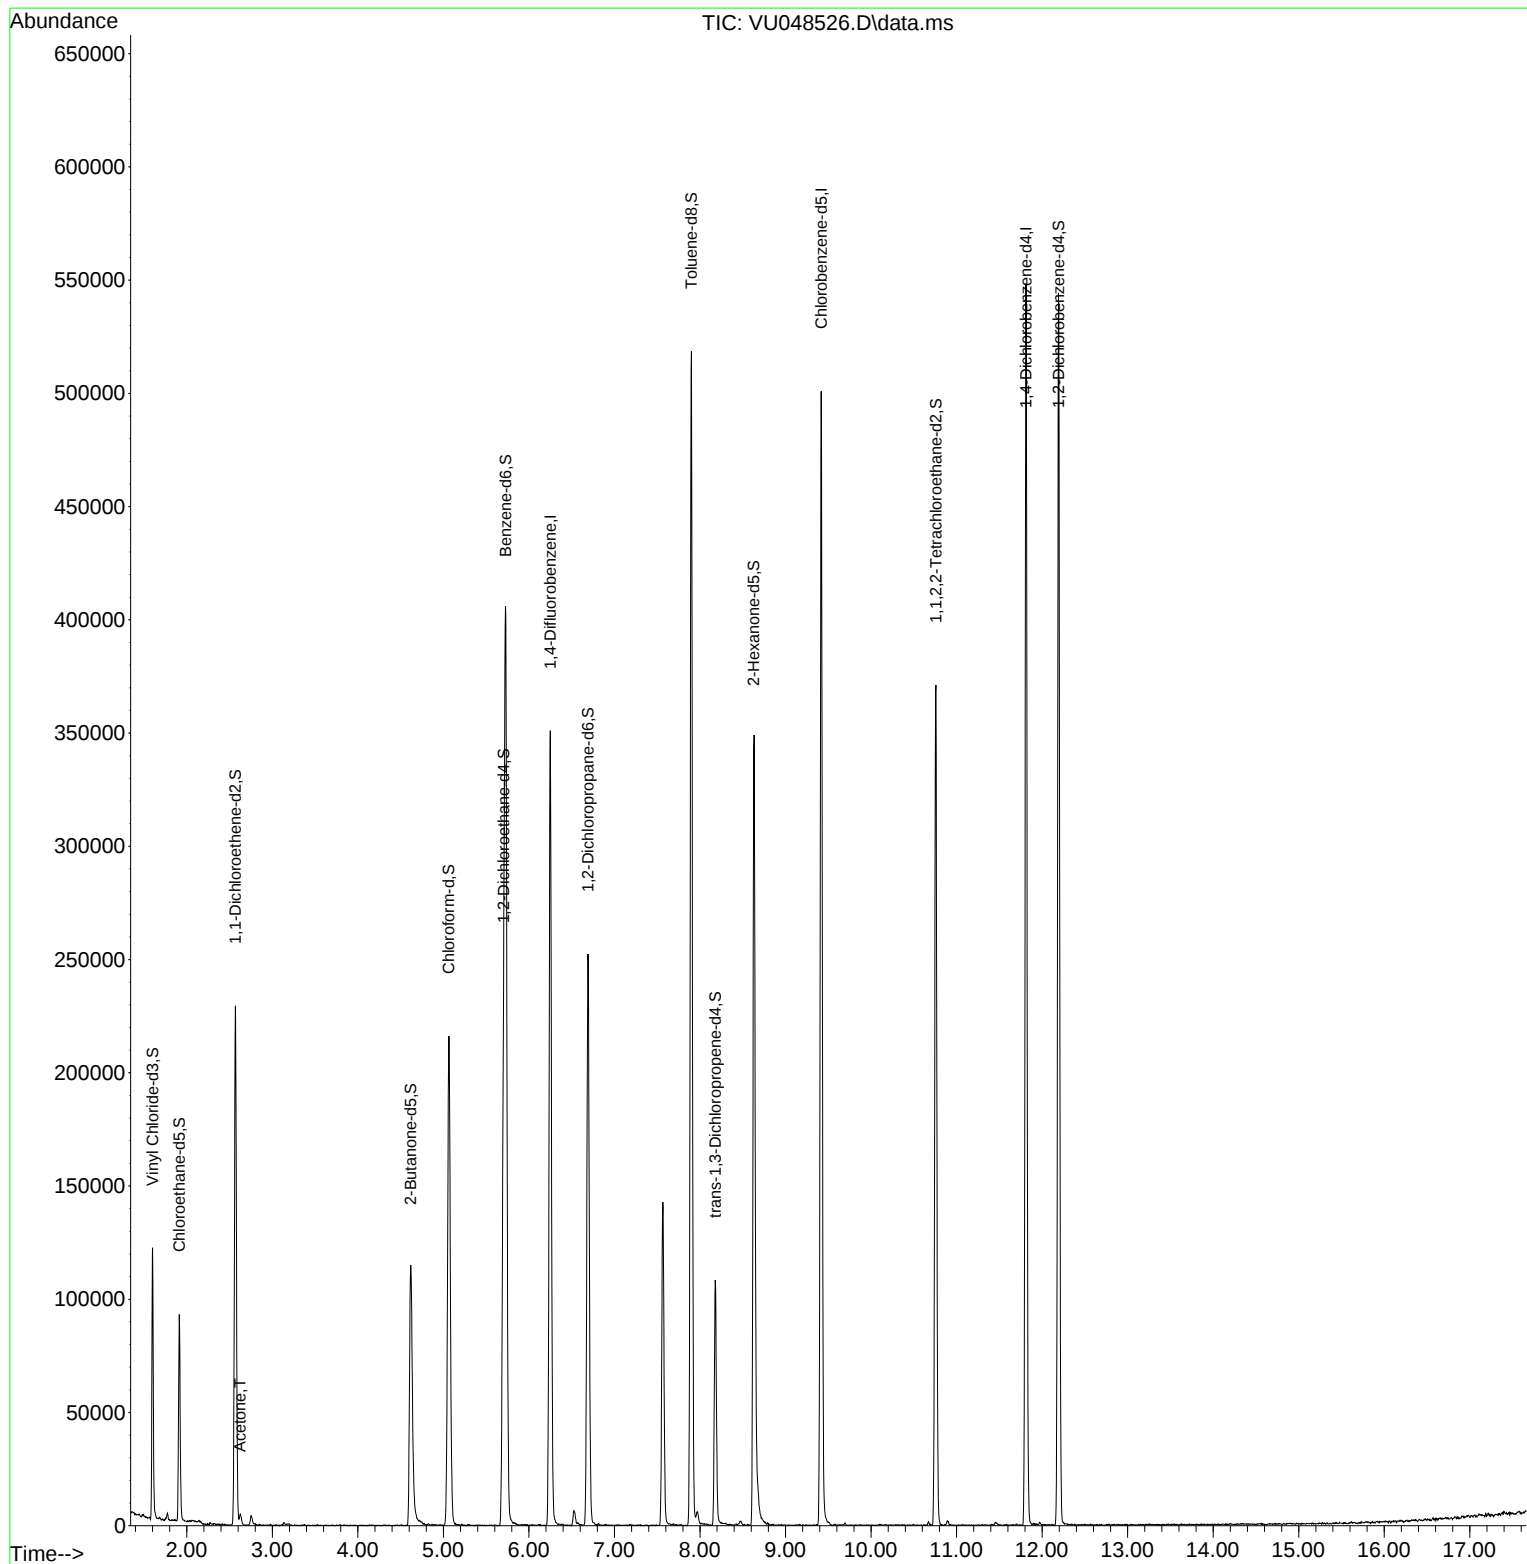

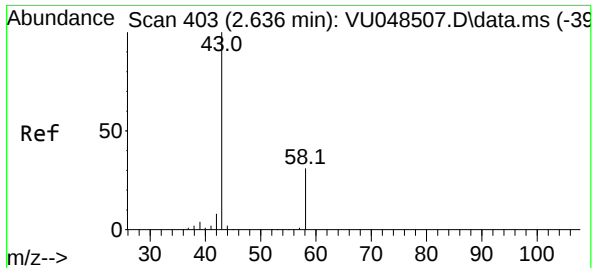

#13
 Acetone
 Concen: 3.372 ug/L
 RT: 2.623 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VU048526.D
 Acq: 11 May 2022 18:48

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP9

Tgt Ion: 43 Resp: 5205
 Ion Ratio Lower Upper
 43 100
 58 27.0 0.0 66.2

