

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048527.D
 Acq On : 11 May 2022 19:12
 Operator : SY/MD
 Sample : N2790-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPPO

Quant Time: May 12 03:45:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 12 03:40:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	262353	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	264192	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	138080	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	78102	34.567	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.140%
7) Chloroethane-d5	1.912	69	62072	42.094	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.180%
11) 1,1-Dichloroethene-d2	2.568	63	130603	32.479	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.960%
21) 2-Butanone-d5	4.620	46	162067	84.225	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.220%
24) Chloroform-d	5.063	84	192355	49.014	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.020%
26) 1,2-Dichloroethane-d4	5.703	65	139417	54.650	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.300%
32) Benzene-d6	5.729	84	355323	44.259	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.520%
36) 1,2-Dichloropropane-d6	6.690	67	108903	41.598	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.200%
41) Toluene-d8	7.899	98	322871	45.473	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.940%
43) trans-1,3-Dichloroprop...	8.179	79	59930	49.736	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.480%
47) 2-Hexanone-d5	8.632	63	120724	95.274	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.270%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	167405	41.979	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.960%
66) 1,2-Dichlorobenzene-d4	12.192	152	139447	51.001	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						
					Qvalue	
13) Acetone	2.633	43	4809	3.315	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048527.D
Acq On : 11 May 2022 19:12
Operator : SY/MD
Sample : N2790-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPPO

Quant Time: May 12 03:45:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 12 03:40:41 2022
Response via : Initial Calibration

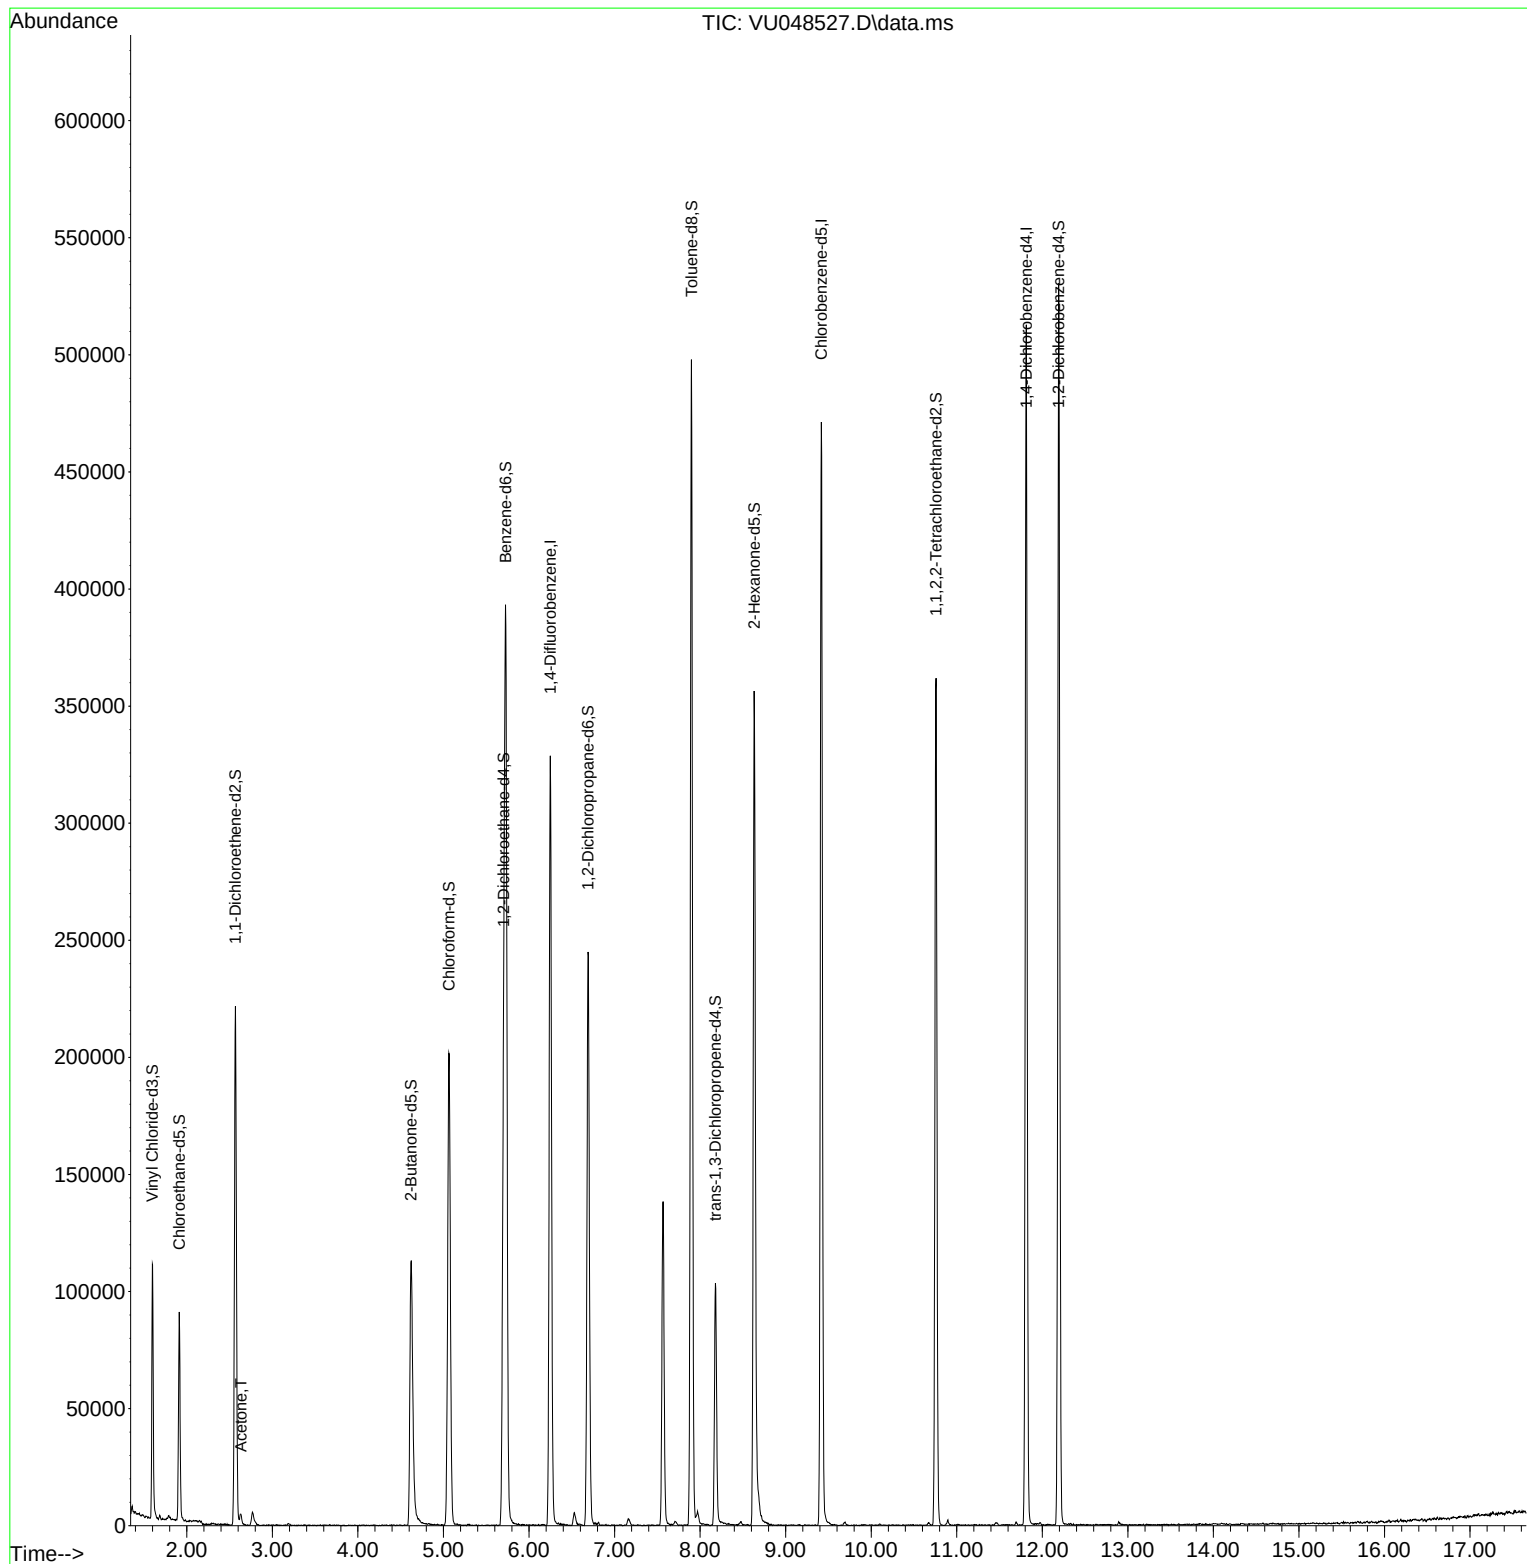

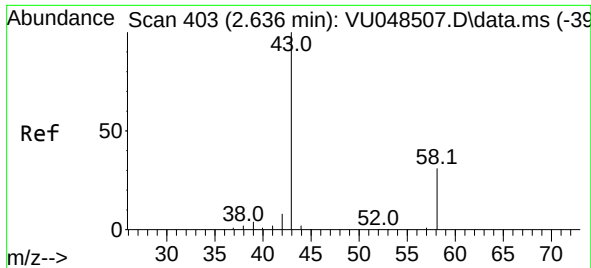

#13
 Acetone
 Concen: 3.315 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU048527.D
 Acq: 11 May 2022 19:12

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPPO

Tgt Ion: 43 Resp: 4809
 Ion Ratio Lower Upper
 43 100
 58 29.4 0.0 66.2

