

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048509.D
 Acq On : 11 May 2022 11:55
 Operator : SY/MD
 Sample : VU0511WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M

Title : VOC Analysis

Signal : TIC: VU048509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rVB	116424	133324	12.59%	1.564%
2	1.912	171	178	195	rVB	88808	114625	10.83%	1.344%
3	2.321	301	305	308	rBV4	691	649	0.06%	0.008%
4	2.485	354	356	363	rVB2	352	274	0.03%	0.003%
5	2.568	370	382	398	rBV	221276	363418	34.32%	4.262%
6	2.690	417	420	426	rBV2	299	278	0.03%	0.003%
7	2.948	497	500	504	rBB2	288	214	0.02%	0.003%
8	3.047	524	531	538	rVB3	1294	1765	0.17%	0.021%
9	3.124	553	555	559	rBV	250	209	0.02%	0.002%
10	3.192	575	576	579	rVB	404	153	0.01%	0.002%
11	3.237	587	590	592	rBV	292	216	0.02%	0.003%
12	3.321	612	616	617	rBV	268	204	0.02%	0.002%
13	3.346	622	624	625	rBV	327	179	0.02%	0.002%
14	3.362	627	629	633	rVB2	193	150	0.01%	0.002%
15	3.472	658	663	666	rBV2	284	288	0.03%	0.003%
16	3.597	700	702	706	rBV	278	209	0.02%	0.002%
17	3.668	720	724	728	rBV	162	210	0.02%	0.002%
18	4.112	860	862	866	rBV	205	179	0.02%	0.002%
19	4.150	872	874	877	rBB	262	147	0.01%	0.002%
20	4.198	885	889	893	rBV2	355	423	0.04%	0.005%
21	4.414	952	956	958	rBV	147	148	0.01%	0.002%
22	4.430	958	961	963	rBV	292	180	0.02%	0.002%
23	4.491	977	980	983	rBV	282	216	0.02%	0.003%
24	4.510	983	986	988	rVV	257	178	0.02%	0.002%
25	4.626	1009	1022	1057	rBV	105023	268635	25.37%	3.150%
26	4.857	1091	1094	1097	rBV3	461	326	0.03%	0.004%
27	5.066	1142	1159	1181	rBV	199061	434373	41.02%	5.094%
28	5.218	1204	1206	1211	rVB2	516	330	0.03%	0.004%
29	5.247	1213	1215	1217	rVB	361	185	0.02%	0.002%
30	5.279	1222	1225	1227	rBV	461	244	0.02%	0.003%
31	5.343	1243	1245	1247	rBB	292	151	0.01%	0.002%
32	5.385	1250	1258	1261	rBV2	357	458	0.04%	0.005%
33	5.430	1268	1272	1274	rBV	345	233	0.02%	0.003%
34	5.446	1274	1277	1279	rBV2	333	244	0.02%	0.003%
35	5.536	1302	1305	1308	rBV	376	285	0.03%	0.003%
36	5.587	1316	1321	1323	rBV2	289	260	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048509.D
 Acq On : 11 May 2022 11:55
 Operator : SY/MD
 Sample : VU0511WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.642	1335	1338	1339	rBV2	273	138	0.01%	0.002%
38	5.726	1342	1364	1395	rVV2	384897	1058823	100.00%	12.417%
39	5.902	1416	1419	1421	rBV	324	205	0.02%	0.002%
40	6.018	1451	1455	1457	rBV2	205	176	0.02%	0.002%
41	6.038	1457	1461	1463	rVV	280	182	0.02%	0.002%
42	6.050	1463	1465	1468	rVB	361	215	0.02%	0.003%
43	6.250	1513	1527	1553	rBV2	346814	655395	61.90%	7.686%
44	6.533	1606	1615	1623	rVB4	3291	5266	0.50%	0.062%
45	6.565	1623	1625	1632	rBV2	330	247	0.02%	0.003%
46	6.693	1650	1665	1688	rBV	242249	469174	44.31%	5.502%
47	6.809	1696	1701	1705	rBV4	921	871	0.08%	0.010%
48	6.935	1736	1740	1746	rBB2	318	375	0.04%	0.004%
49	6.967	1747	1750	1752	rBV	244	178	0.02%	0.002%
50	7.034	1767	1771	1772	rBV	311	192	0.02%	0.002%
51	7.121	1797	1798	1803	rVB	430	245	0.02%	0.003%
52	7.160	1806	1810	1813	rBV2	299	305	0.03%	0.004%
53	7.189	1816	1819	1821	rVV3	307	212	0.02%	0.002%
54	7.221	1827	1829	1833	rVB2	257	166	0.02%	0.002%
55	7.256	1838	1840	1845	rVB	233	172	0.02%	0.002%
56	7.375	1874	1877	1878	rBV	224	157	0.01%	0.002%
57	7.568	1924	1937	1955	rBV2	140523	248797	23.50%	2.918%
58	7.767	1996	1999	2000	rBV	400	276	0.03%	0.003%
59	7.803	2005	2010	2015	rVV2	523	475	0.04%	0.006%
60	7.899	2026	2040	2056	rBV	482536	843502	79.66%	9.892%
61	8.047	2083	2086	2090	rBV3	483	357	0.03%	0.004%
62	8.121	2106	2109	2112	rVB	254	156	0.01%	0.002%
63	8.179	2115	2127	2144	rBV	100229	177220	16.74%	2.078%
64	8.462	2211	2215	2216	rBV	641	354	0.03%	0.004%
65	8.549	2237	2242	2245	rBV	245	303	0.03%	0.004%
66	8.635	2257	2269	2298	rBV	341103	615890	58.17%	7.223%
67	8.854	2334	2337	2342	rBV2	317	299	0.03%	0.004%
68	8.902	2346	2352	2354	rBV	319	323	0.03%	0.004%
69	9.005	2380	2384	2386	rBV	319	280	0.03%	0.003%
70	9.073	2402	2405	2407	rBV2	269	159	0.02%	0.002%
71	9.253	2458	2461	2465	rVB	274	153	0.01%	0.002%
72	9.417	2500	2512	2538	rBV	501549	836939	79.04%	9.815%
73	9.645	2580	2583	2587	rBV3	346	266	0.03%	0.003%
74	9.803	2628	2632	2637	rBV	320	293	0.03%	0.003%
75	9.899	2658	2662	2666	rBV2	382	271	0.03%	0.003%
76	9.934	2669	2673	2678	rVV	301	259	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048509.D
 Acq On : 11 May 2022 11:55
 Operator : SY/MD
 Sample : VU0511WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.362	2804	2806	2810	rBV2	333	228	0.02%	0.003%
78	10.671	2898	2902	2910	rVB4	1940	2384	0.23%	0.028%
79	10.758	2916	2929	2949	rBV	346394	559490	52.84%	6.561%
80	10.832	2950	2952	2955	rVB	477	195	0.02%	0.002%
81	10.860	2958	2961	2962	rBV2	331	142	0.01%	0.002%
82	11.137	3045	3047	3049	rVB	381	141	0.01%	0.002%
83	11.378	3119	3122	3124	rBV	322	169	0.02%	0.002%
84	11.417	3132	3134	3137	rVB2	375	197	0.02%	0.002%
85	11.526	3164	3168	3169	rBV	286	206	0.02%	0.002%
86	11.552	3174	3176	3180	rVB2	316	193	0.02%	0.002%
87	11.584	3180	3186	3189	rBV2	515	532	0.05%	0.006%
88	11.655	3204	3208	3211	rVB2	391	293	0.03%	0.003%
89	11.690	3216	3219	3221	rBV3	807	568	0.05%	0.007%
90	11.751	3232	3238	3241	rBV2	1082	914	0.09%	0.011%
91	11.812	3245	3257	3278	rVV	546434	873644	82.51%	10.245%
92	12.192	3362	3375	3394	rBV	517480	839362	79.27%	9.843%
93	12.365	3426	3429	3432	rBV2	250	189	0.02%	0.002%
94	12.430	3447	3449	3453	rVB	345	177	0.02%	0.002%
95	12.497	3467	3470	3473	rBV2	280	244	0.02%	0.003%
96	12.632	3509	3512	3513	rBV2	277	147	0.01%	0.002%
97	13.166	3674	3678	3681	rBV	420	333	0.03%	0.004%
98	13.282	3711	3714	3717	rBV	343	230	0.02%	0.003%
99	14.095	3959	3967	3969	rBV2	2101	2685	0.25%	0.031%
100	14.327	4036	4039	4053	rVB7	1128	1733	0.16%	0.020%




Sum of corrected areas: 8527222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048509.D
Acq On : 11 May 2022 11:55
Operator : SY/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

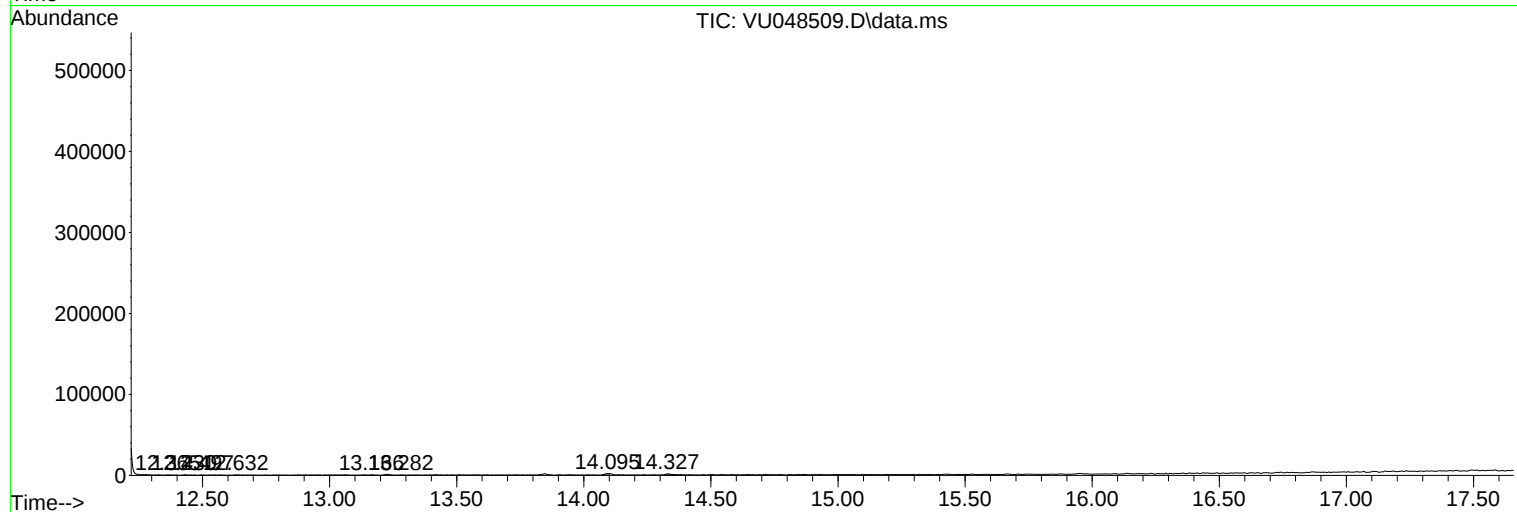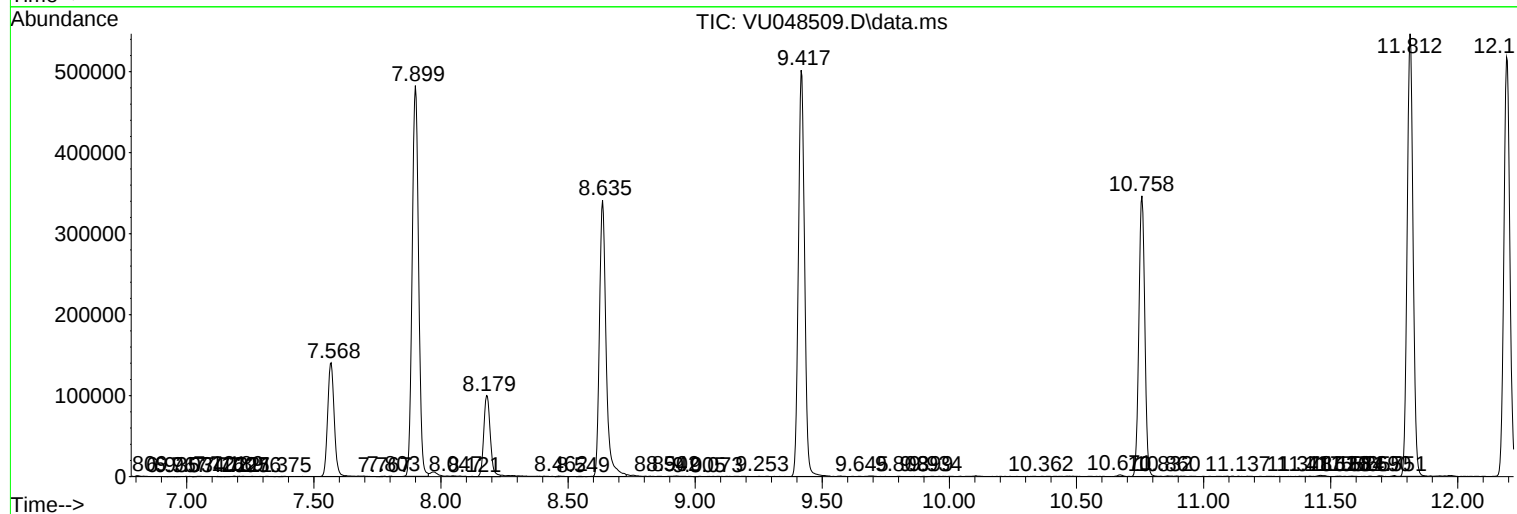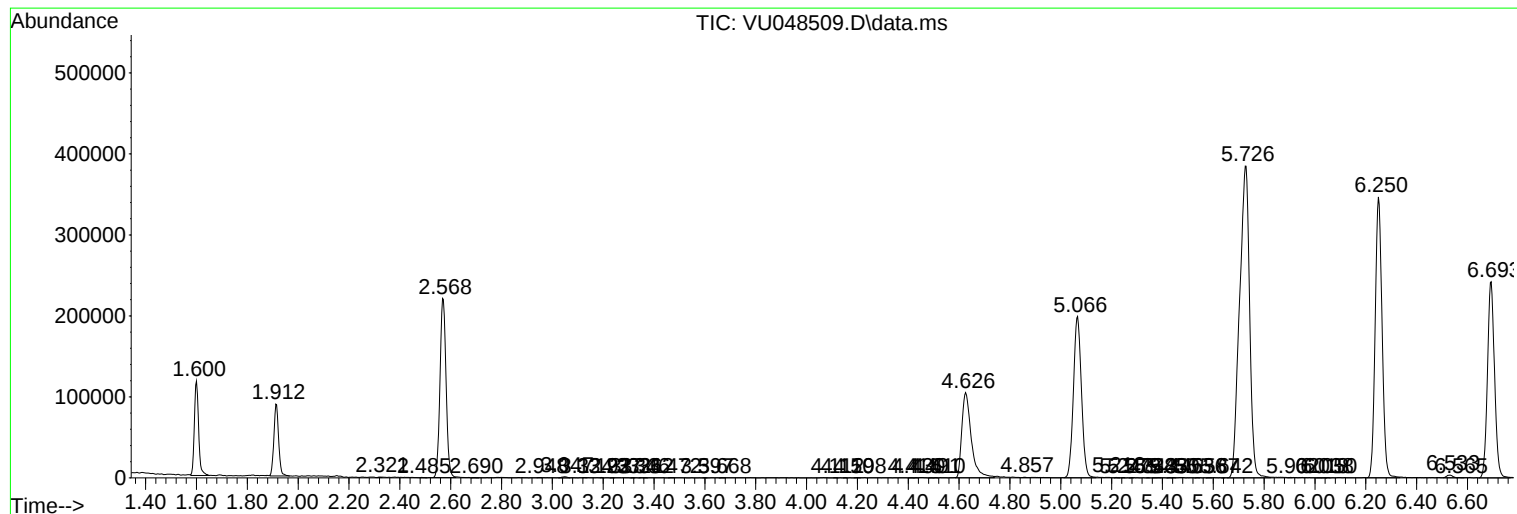

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048509.D
Acq On : 11 May 2022 11:55
Operator : SY/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048509.D
Acq On : 11 May 2022 11:55
Operator : SY/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------