

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048511.D
 Acq On : 11 May 2022 12:43
 Operator : SY/MD
 Sample : N2736-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	88797	99038	10.06%	1.236%
2	1.912	170	178	193	rVB	76957	101408	10.30%	1.265%
3	2.568	368	382	393	rBV	186940	304287	30.90%	3.797%
4	2.790	449	451	460	rVB2	436	394	0.04%	0.005%
5	2.861	470	473	476	rBV2	239	185	0.02%	0.002%
6	2.893	479	483	486	rBV2	824	743	0.08%	0.009%
7	3.012	516	520	525	rVB2	364	398	0.04%	0.005%
8	3.050	526	532	536	rBV3	483	470	0.05%	0.006%
9	3.163	562	567	568	rBV2	895	723	0.07%	0.009%
10	3.279	602	603	607	rBV	237	176	0.02%	0.002%
11	3.321	613	616	620	rVB2	301	187	0.02%	0.002%
12	3.517	675	677	681	rBV2	339	261	0.03%	0.003%
13	3.539	681	684	688	rVV2	320	286	0.03%	0.004%
14	3.587	689	699	703	rVB2	760	910	0.09%	0.011%
15	3.661	720	722	726	rBB	255	188	0.02%	0.002%
16	3.687	727	730	732	rBV	392	254	0.03%	0.003%
17	3.764	748	754	761	rBB	285	424	0.04%	0.005%
18	4.089	852	855	857	rBV	225	175	0.02%	0.002%
19	4.227	894	898	901	rBV	272	251	0.03%	0.003%
20	4.433	956	962	967	rVB2	528	577	0.06%	0.007%
21	4.549	986	998	1000	rBV2	2331	3094	0.31%	0.039%
22	4.620	1008	1020	1047	rBV	110964	259587	26.36%	3.239%
23	4.835	1085	1087	1090	rBV2	374	264	0.03%	0.003%
24	4.886	1101	1103	1107	rBV3	264	198	0.02%	0.002%
25	5.063	1143	1158	1183	rBV	189370	419301	42.57%	5.232%
26	5.227	1203	1209	1210	rBV	309	324	0.03%	0.004%
27	5.285	1225	1227	1231	rBV	528	395	0.04%	0.005%
28	5.324	1234	1239	1241	rBV2	328	333	0.03%	0.004%
29	5.385	1255	1258	1263	rBV2	345	345	0.04%	0.004%
30	5.414	1263	1267	1268	rBV	298	194	0.02%	0.002%
31	5.472	1281	1285	1288	rBV2	310	268	0.03%	0.003%
32	5.533	1300	1304	1307	rBV	334	324	0.03%	0.004%
33	5.626	1331	1333	1337	rBB	257	206	0.02%	0.003%
34	5.726	1341	1364	1391	rBV2	355711	984876	100.00%	12.288%
35	5.951	1430	1434	1436	rBV2	396	288	0.03%	0.004%
36	6.037	1456	1461	1462	rBV	464	410	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048511.D
 Acq On : 11 May 2022 12:43
 Operator : SY/MD
 Sample : N2736-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	6.111	1481	1484	1486	rBV2	365	190	0.02%	0.002%
38	6.250	1513	1527	1549	rBV	332362	628310	63.80%	7.839%
39	6.401	1570	1574	1579	rVB3	463	456	0.05%	0.006%
40	6.436	1579	1585	1587	rBV	364	343	0.03%	0.004%
41	6.449	1587	1589	1595	rVV2	332	328	0.03%	0.004%
42	6.481	1595	1599	1602	rVB2	434	347	0.04%	0.004%
43	6.526	1604	1613	1624	rVB3	4692	7939	0.81%	0.099%
44	6.581	1625	1630	1633	rVB2	443	371	0.04%	0.005%
45	6.610	1634	1639	1640	rBV	357	260	0.03%	0.003%
46	6.690	1651	1664	1688	rBV	224840	444610	45.14%	5.547%
47	6.806	1697	1700	1705	rBV4	692	679	0.07%	0.008%
48	6.870	1716	1720	1721	rBV	285	206	0.02%	0.003%
49	6.954	1744	1746	1749	rBV	274	216	0.02%	0.003%
50	6.980	1751	1754	1758	rVB2	238	189	0.02%	0.002%
51	7.041	1770	1773	1775	rVB2	337	214	0.02%	0.003%
52	7.054	1775	1777	1780	rVB2	392	225	0.02%	0.003%
53	7.079	1782	1785	1789	rVB2	319	197	0.02%	0.002%
54	7.111	1789	1795	1798	rVB2	485	590	0.06%	0.007%
55	7.185	1810	1818	1824	rBV3	1974	2955	0.30%	0.037%
56	7.250	1836	1838	1846	rVB2	336	442	0.04%	0.006%
57	7.285	1846	1849	1852	rBV	399	291	0.03%	0.004%
58	7.565	1924	1936	1955	rBV	126830	225216	22.87%	2.810%
59	7.677	1968	1971	1972	rBV	678	402	0.04%	0.005%
60	7.835	2018	2020	2024	rVB	441	255	0.03%	0.003%
61	7.899	2024	2040	2056	rBV	440168	754677	76.63%	9.416%
62	8.115	2104	2107	2111	rBV2	235	169	0.02%	0.002%
63	8.179	2116	2127	2144	rBV	95267	164498	16.70%	2.052%
64	8.513	2228	2231	2235	rVB	306	281	0.03%	0.004%
65	8.632	2254	2268	2298	rBV	337030	608408	61.78%	7.591%
66	8.880	2341	2345	2348	rBV2	369	235	0.02%	0.003%
67	8.934	2352	2362	2367	rBV2	472	623	0.06%	0.008%
68	8.976	2367	2375	2377	rBV	327	369	0.04%	0.005%
69	9.063	2399	2402	2404	rBV	254	174	0.02%	0.002%
70	9.098	2410	2413	2416	rBV2	209	176	0.02%	0.002%
71	9.118	2416	2419	2422	rVB2	297	188	0.02%	0.002%
72	9.301	2471	2476	2478	rBV2	254	269	0.03%	0.003%
73	9.336	2483	2487	2490	rBV2	401	417	0.04%	0.005%
74	9.417	2498	2512	2551	rBV	484420	797760	81.00%	9.954%
75	9.690	2595	2597	2604	rVB2	520	467	0.05%	0.006%
76	10.433	2825	2828	2830	rBV	358	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048511.D
 Acq On : 11 May 2022 12:43
 Operator : SY/MD
 Sample : N2736-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXEX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.668	2896	2901	2909	rVB5	1135	1334	0.14%	0.017%
78	10.758	2913	2929	2947	rBV	348041	559989	56.86%	6.987%
79	10.893	2966	2971	2982	rVB2	1633	2515	0.26%	0.031%
80	10.934	2982	2984	2986	rBV	339	167	0.02%	0.002%
81	10.999	3001	3004	3008	rVB	279	166	0.02%	0.002%
82	11.082	3028	3030	3034	rBV	323	225	0.02%	0.003%
83	11.201	3064	3067	3071	rBV2	270	214	0.02%	0.003%
84	11.253	3080	3083	3086	rBV	301	172	0.02%	0.002%
85	11.465	3140	3149	3158	rBV4	870	1965	0.20%	0.025%
86	11.700	3217	3222	3224	rBV2	390	323	0.03%	0.004%
87	11.812	3243	3257	3274	rBV	526970	833324	84.61%	10.397%
88	11.902	3283	3285	3289	rBV2	591	376	0.04%	0.005%
89	11.963	3302	3304	3307	rBV2	439	345	0.04%	0.004%
90	12.057	3329	3333	3335	rBV3	434	325	0.03%	0.004%
91	12.192	3363	3375	3392	rBV	481304	784277	79.63%	9.785%
92	12.513	3472	3475	3480	rVB2	492	372	0.04%	0.005%
93	12.851	3577	3580	3583	rBV	278	175	0.02%	0.002%
94	13.018	3628	3632	3634	rBV2	305	203	0.02%	0.003%
95	13.063	3643	3646	3651	rBV3	507	428	0.04%	0.005%
96	13.092	3651	3655	3656	rBV	224	172	0.02%	0.002%
97	13.188	3683	3685	3687	rBV	333	197	0.02%	0.002%
98	13.915	3908	3911	3917	rBV2	367	361	0.04%	0.005%
99	13.957	3921	3924	3926	rBV	383	215	0.02%	0.003%
100	15.677	4455	4459	4463	rBV4	900	1028	0.10%	0.013%




Sum of corrected areas: 8014738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048511.D
Acq On : 11 May 2022 12:43
Operator : SY/MD
Sample : N2736-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

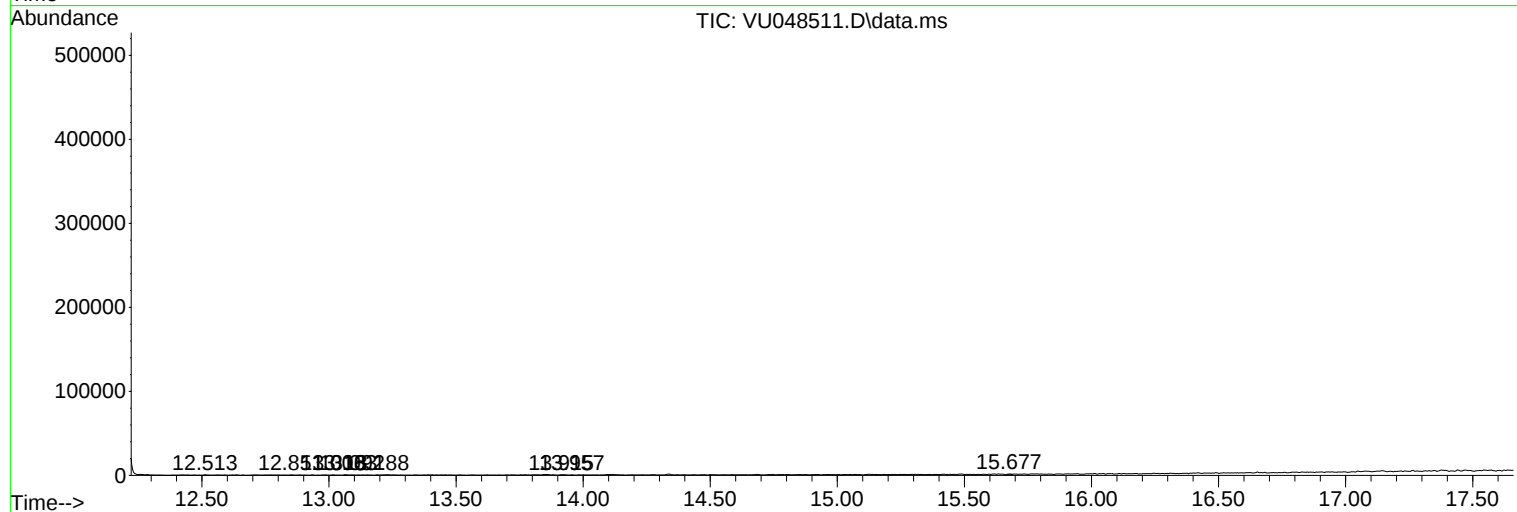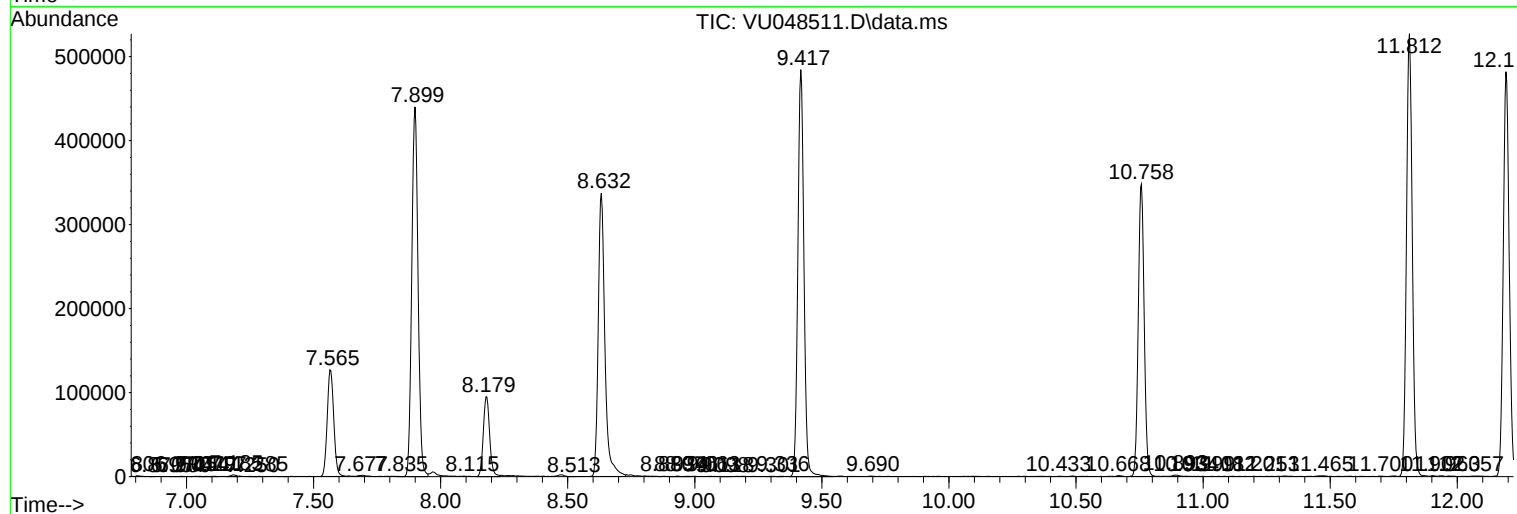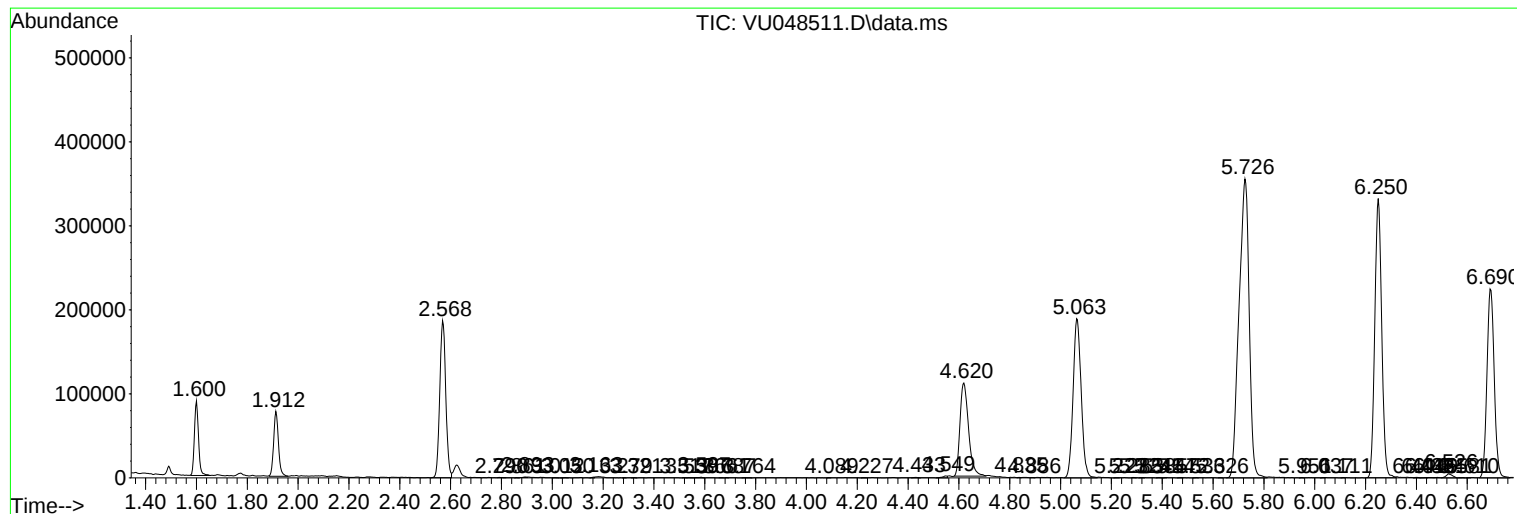

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048511.D
Acq On : 11 May 2022 12:43
Operator : SY/MD
Sample : N2736-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048511.D
Acq On : 11 May 2022 12:43
Operator : SY/MD
Sample : N2736-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXEX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------