

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048514.D
 Acq On : 11 May 2022 14:09
 Operator : SY/MD
 Sample : N2790-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	124022	137256	12.16%	1.576%
2	1.912	170	178	193	rBV	91880	118374	10.49%	1.359%
3	2.568	370	382	397	rBV	234311	382651	33.91%	4.393%
4	3.041	526	529	531	rBV	215	136	0.01%	0.002%
5	3.092	543	545	547	rBV	255	143	0.01%	0.002%
6	3.182	562	573	582	rBV4	4024	7703	0.68%	0.088%
7	3.263	594	598	604	rBB	450	509	0.05%	0.006%
8	3.324	614	617	620	rBV	277	218	0.02%	0.003%
9	3.385	632	636	637	rBV	172	143	0.01%	0.002%
10	3.568	688	693	696	rBV	236	227	0.02%	0.003%
11	3.800	762	765	768	rBB	339	247	0.02%	0.003%
12	3.848	777	780	784	rVB2	255	207	0.02%	0.002%
13	4.131	866	868	872	rBB	382	250	0.02%	0.003%
14	4.157	873	876	879	rBV	185	172	0.02%	0.002%
15	4.179	880	883	887	rVV2	259	259	0.02%	0.003%
16	4.208	890	892	897	rBB2	251	172	0.02%	0.002%
17	4.237	898	901	905	rBV	180	205	0.02%	0.002%
18	4.440	961	964	967	rBV	237	185	0.02%	0.002%
19	4.520	985	989	991	rBV2	301	226	0.02%	0.003%
20	4.565	1000	1003	1004	rBV	237	148	0.01%	0.002%
21	4.620	1008	1020	1045	rBV	116339	279320	24.75%	3.207%
22	5.063	1136	1158	1180	rBV	212213	466961	41.38%	5.361%
23	5.202	1193	1201	1205	rBV3	640	655	0.06%	0.008%
24	5.227	1206	1209	1214	rBV2	288	231	0.02%	0.003%
25	5.298	1228	1231	1232	rBV2	372	234	0.02%	0.003%
26	5.343	1241	1245	1247	rBV	339	204	0.02%	0.002%
27	5.372	1252	1254	1257	rBV	228	182	0.02%	0.002%
28	5.430	1269	1272	1273	rBV	217	147	0.01%	0.002%
29	5.462	1278	1282	1284	rBV	216	193	0.02%	0.002%
30	5.584	1317	1320	1323	rBB2	243	165	0.01%	0.002%
31	5.652	1337	1341	1343	rBV	305	266	0.02%	0.003%
32	5.726	1343	1364	1390	rVV2	416028	1128444	100.00%	12.955%
33	5.973	1438	1441	1443	rVB2	357	217	0.02%	0.002%
34	5.989	1443	1446	1449	rBV3	389	260	0.02%	0.003%
35	6.031	1456	1459	1460	rBV	326	140	0.01%	0.002%
36	6.076	1471	1473	1476	rVB2	297	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048514.D
 Acq On : 11 May 2022 14:09
 Operator : SY/MD
 Sample : N2790-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	6.099	1476	1480	1483	rBB2	325	269	0.02%	0.003%
38	6.121	1484	1487	1490	rBV2	568	535	0.05%	0.006%
39	6.186	1501	1507	1512	rBV2	200	321	0.03%	0.004%
40	6.250	1512	1527	1549	rBV	318259	598415	53.03%	6.870%
41	6.459	1588	1592	1593	rBV	283	170	0.02%	0.002%
42	6.533	1604	1615	1628	rVB4	4915	8979	0.80%	0.103%
43	6.690	1650	1664	1686	rBV	256796	499294	44.25%	5.732%
44	6.848	1711	1713	1715	rBV	288	156	0.01%	0.002%
45	7.018	1761	1766	1768	rBV	197	184	0.02%	0.002%
46	7.044	1772	1774	1777	rVV	251	163	0.01%	0.002%
47	7.076	1781	1784	1787	rBV2	166	139	0.01%	0.002%
48	7.182	1815	1817	1825	rVB2	816	704	0.06%	0.008%
49	7.250	1833	1838	1839	rBV	286	244	0.02%	0.003%
50	7.346	1864	1868	1872	rBB2	493	362	0.03%	0.004%
51	7.369	1872	1875	1878	rBV	274	207	0.02%	0.002%
52	7.407	1884	1887	1889	rBV	295	229	0.02%	0.003%
53	7.443	1893	1898	1903	rBV	197	228	0.02%	0.003%
54	7.468	1903	1906	1908	rBV	291	159	0.01%	0.002%
55	7.565	1923	1936	1957	rBV	149575	264972	23.48%	3.042%
56	7.652	1960	1963	1965	rBV3	552	335	0.03%	0.004%
57	7.748	1989	1993	1994	rBV3	268	144	0.01%	0.002%
58	7.780	1999	2003	2006	rBV	299	270	0.02%	0.003%
59	7.848	2021	2024	2026	rBV	224	141	0.01%	0.002%
60	7.899	2026	2040	2057	rBV	530777	902645	79.99%	10.362%
61	8.179	2114	2127	2147	rBV	108528	187524	16.62%	2.153%
62	8.475	2213	2219	2229	rVB6	1845	3039	0.27%	0.035%
63	8.539	2236	2239	2241	rBV	272	163	0.01%	0.002%
64	8.632	2255	2268	2293	rBV	365956	642541	56.94%	7.376%
65	8.838	2330	2332	2335	rVB2	312	190	0.02%	0.002%
66	8.973	2371	2374	2376	rBV2	286	211	0.02%	0.002%
67	8.996	2376	2381	2384	rVV2	220	225	0.02%	0.003%
68	9.156	2428	2431	2432	rBV	250	136	0.01%	0.002%
69	9.275	2464	2468	2470	rBV	285	246	0.02%	0.003%
70	9.417	2499	2512	2534	rBV	456046	755170	66.92%	8.669%
71	9.562	2556	2557	2560	rBV	225	145	0.01%	0.002%
72	9.690	2592	2597	2604	rBV2	767	931	0.08%	0.011%
73	9.777	2621	2624	2627	rVB2	316	145	0.01%	0.002%
74	9.957	2677	2680	2682	rBV2	288	194	0.02%	0.002%
75	10.076	2714	2717	2721	rBV2	199	144	0.01%	0.002%
76	10.102	2722	2725	2726	rBV	333	183	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048514.D
 Acq On : 11 May 2022 14:09
 Operator : SY/MD
 Sample : N2790-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.478	2839	2842	2843	rBV	344	170	0.02%	0.002%
78	10.536	2857	2860	2863	rBV2	289	231	0.02%	0.003%
79	10.671	2895	2902	2910	rBV6	1984	2563	0.23%	0.029%
80	10.754	2916	2928	2949	rVB	367173	600258	53.19%	6.891%
81	10.841	2953	2955	2958	rVV2	312	181	0.02%	0.002%
82	10.864	2960	2962	2964	rVV2	457	262	0.02%	0.003%
83	10.896	2964	2972	2981	rVB2	2620	4110	0.36%	0.047%
84	10.954	2987	2990	2993	rVB2	215	137	0.01%	0.002%
85	10.973	2993	2996	2997	rBV2	269	138	0.01%	0.002%
86	11.086	3028	3031	3034	rBV2	457	270	0.02%	0.003%
87	11.282	3089	3092	3094	rBV	244	176	0.02%	0.002%
88	11.812	3244	3257	3273	rBV	505146	793865	70.35%	9.114%
89	11.928	3290	3293	3299	rBV4	619	696	0.06%	0.008%
90	12.034	3322	3326	3328	rBV	248	181	0.02%	0.002%
91	12.076	3337	3339	3342	rBV2	426	234	0.02%	0.003%
92	12.192	3362	3375	3393	rBV	548291	885061	78.43%	10.161%
93	12.352	3423	3425	3428	rVB	331	156	0.01%	0.002%
94	12.401	3436	3440	3445	rBV	250	194	0.02%	0.002%
95	12.426	3445	3448	3449	rBV	380	202	0.02%	0.002%
96	12.774	3551	3556	3559	rBV3	522	431	0.04%	0.005%
97	13.015	3621	3631	3648	rBV3	11994	22545	2.00%	0.259%
98	13.108	3656	3660	3665	rBV4	541	529	0.05%	0.006%
99	13.304	3719	3721	3723	rBV	234	136	0.01%	0.002%
100	13.430	3754	3760	3764	rBV2	285	353	0.03%	0.004%




Sum of corrected areas: 8710763

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048514.D
Acq On : 11 May 2022 14:09
Operator : SY/MD
Sample : N2790-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

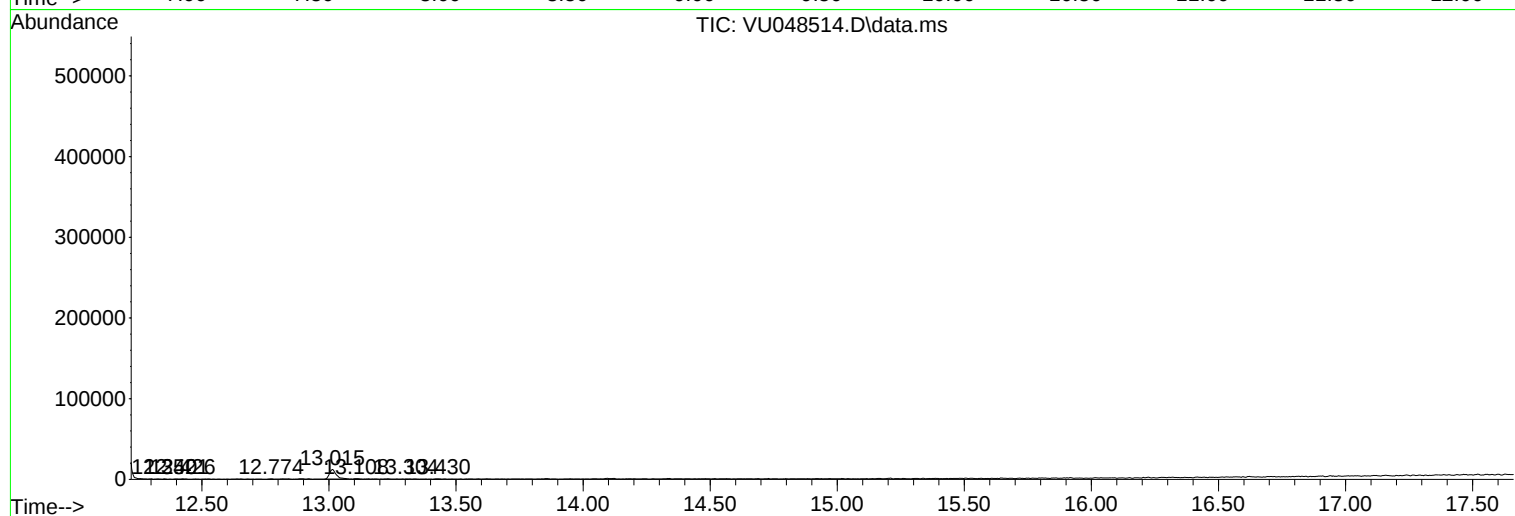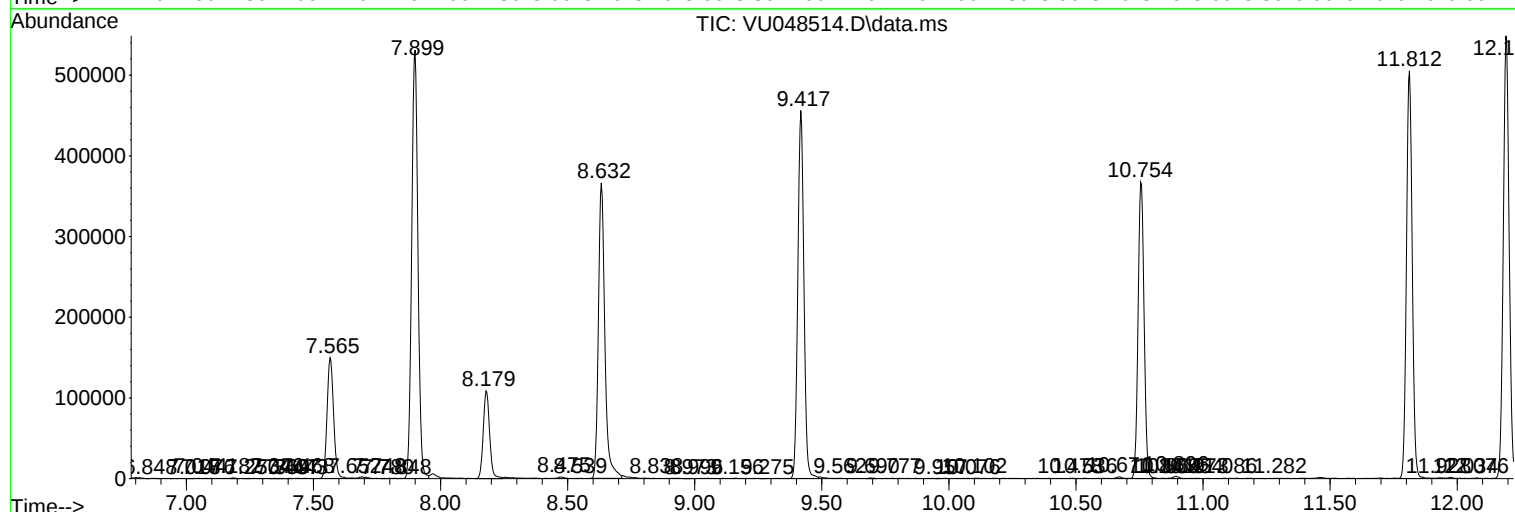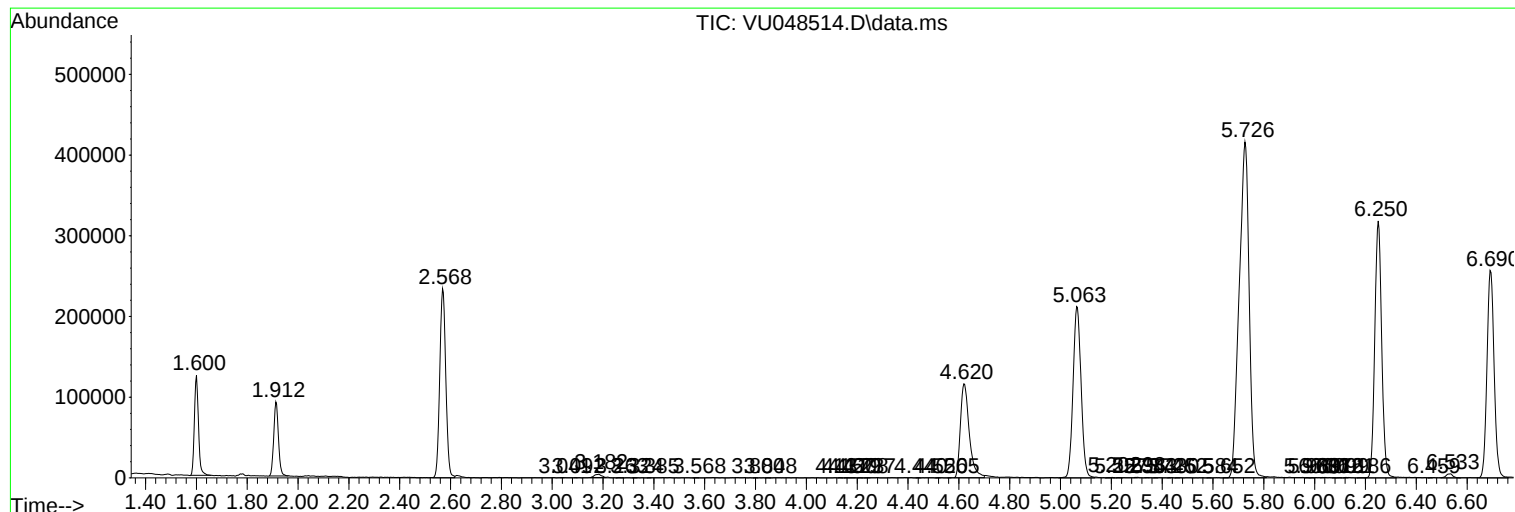

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048514.D
Acq On : 11 May 2022 14:09
Operator : SY/MD
Sample : N2790-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048514.D
Acq On : 11 May 2022 14:09
Operator : SY/MD
Sample : N2790-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc