

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048518.D
 Acq On : 11 May 2022 15:42
 Operator : SY/MD
 Sample : N2790-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGNP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	128728	146906	12.36%	1.565%
2	1.912	170	178	191	rBV	96383	124023	10.43%	1.321%
3	2.568	369	382	395	rBV	251784	402448	33.85%	4.287%
4	2.758	431	441	455	rBV	7144	13650	1.15%	0.145%
5	2.928	491	494	496	rVB2	284	187	0.02%	0.002%
6	2.954	497	502	503	rBV2	378	301	0.03%	0.003%
7	3.041	524	529	530	rBV2	789	586	0.05%	0.006%
8	3.073	537	539	543	rVB2	313	223	0.02%	0.002%
9	3.099	543	547	549	rBV	222	195	0.02%	0.002%
10	3.137	556	559	562	rBV2	326	278	0.02%	0.003%
11	3.189	568	575	578	rBV2	685	907	0.08%	0.010%
12	3.237	587	590	592	rBV2	229	152	0.01%	0.002%
13	3.327	615	618	621	rBV	267	234	0.02%	0.002%
14	3.462	656	660	662	rBV2	231	173	0.01%	0.002%
15	3.835	773	776	780	rVB	298	229	0.02%	0.002%
16	3.919	796	802	804	rBV	303	286	0.02%	0.003%
17	4.025	831	835	838	rBV	198	206	0.02%	0.002%
18	4.067	845	848	852	rBV	212	203	0.02%	0.002%
19	4.150	871	874	877	rBB	218	152	0.01%	0.002%
20	4.192	883	887	893	rBB	351	342	0.03%	0.004%
21	4.234	894	900	903	rBB2	330	337	0.03%	0.004%
22	4.334	925	931	934	rBV	243	245	0.02%	0.003%
23	4.407	951	954	956	rBV	180	139	0.01%	0.001%
24	4.465	970	972	975	rVB2	243	151	0.01%	0.002%
25	4.543	990	996	999	rBV2	354	383	0.03%	0.004%
26	4.620	1005	1020	1046	rBV	125353	300132	25.25%	3.197%
27	5.067	1142	1159	1187	rBV2	231961	566967	47.69%	6.040%
28	5.211	1200	1204	1209	rBV3	569	621	0.05%	0.007%
29	5.234	1209	1211	1214	rVB2	284	177	0.01%	0.002%
30	5.279	1222	1225	1226	rBV	440	207	0.02%	0.002%
31	5.317	1235	1237	1239	rBV	268	140	0.01%	0.001%
32	5.333	1239	1242	1245	rVB2	220	172	0.01%	0.002%
33	5.375	1253	1255	1258	rBV2	247	140	0.01%	0.001%
34	5.475	1282	1286	1289	rBV2	266	241	0.02%	0.003%
35	5.497	1291	1293	1296	rBB	308	185	0.02%	0.002%
36	5.620	1329	1331	1334	rVB	302	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048518.D
 Acq On : 11 May 2022 15:42
 Operator : SY/MD
 Sample : N2790-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.649	1335	1340	1342	rBB	171	136	0.01%	0.001%
38	5.726	1343	1364	1392	rBV2	428143	1188755	100.00%	12.664%
39	5.919	1422	1424	1426	rBV	244	138	0.01%	0.001%
40	5.980	1440	1443	1447	rBV2	348	310	0.03%	0.003%
41	6.092	1475	1478	1480	rBV2	406	242	0.02%	0.003%
42	6.112	1480	1484	1491	rVV2	439	423	0.04%	0.005%
43	6.141	1491	1493	1496	rBV	289	215	0.02%	0.002%
44	6.250	1511	1527	1552	rBV	353326	662169	55.70%	7.054%
45	6.388	1567	1570	1573	rBV2	318	308	0.03%	0.003%
46	6.465	1590	1594	1598	rBV2	251	264	0.02%	0.003%
47	6.526	1605	1613	1624	rBV6	5655	9993	0.84%	0.106%
48	6.610	1637	1639	1648	rVB2	568	587	0.05%	0.006%
49	6.690	1649	1664	1682	rBV	268142	526131	44.26%	5.605%
50	6.800	1696	1698	1700	rBV	474	316	0.03%	0.003%
51	6.906	1728	1731	1734	rBV2	177	140	0.01%	0.001%
52	6.944	1738	1743	1746	rBV	178	184	0.02%	0.002%
53	6.983	1753	1755	1758	rVB	416	173	0.01%	0.002%
54	7.018	1763	1766	1769	rVB2	351	246	0.02%	0.003%
55	7.054	1769	1777	1778	rBV3	663	768	0.06%	0.008%
56	7.124	1796	1799	1800	rBV3	351	181	0.02%	0.002%
57	7.157	1803	1809	1815	rBV6	1924	3056	0.26%	0.033%
58	7.250	1833	1838	1840	rBV2	303	272	0.02%	0.003%
59	7.327	1858	1862	1864	rBV	323	278	0.02%	0.003%
60	7.394	1880	1883	1886	rBV2	296	242	0.02%	0.003%
61	7.475	1905	1908	1910	rBV	202	136	0.01%	0.001%
62	7.565	1923	1936	1962	rBV	156642	278618	23.44%	2.968%
63	7.767	1997	1999	2003	rBV	257	170	0.01%	0.002%
64	7.899	2023	2040	2055	rBV	549104	951849	80.07%	10.140%
65	8.115	2104	2107	2111	rBB2	353	314	0.03%	0.003%
66	8.179	2112	2127	2147	rBV	117141	198591	16.71%	2.116%
67	8.394	2191	2194	2196	rBV	687	415	0.03%	0.004%
68	8.552	2237	2243	2248	rVB5	1468	1437	0.12%	0.015%
69	8.632	2256	2268	2300	rBV	386092	691310	58.15%	7.365%
70	8.825	2326	2328	2331	rBV	240	185	0.02%	0.002%
71	8.922	2356	2358	2365	rVB2	463	344	0.03%	0.004%
72	9.211	2444	2448	2449	rBV	392	206	0.02%	0.002%
73	9.417	2499	2512	2547	rBV	501877	837839	70.48%	8.925%
74	9.562	2554	2557	2565	rBV2	660	802	0.07%	0.009%
75	9.616	2571	2574	2580	rBV2	297	215	0.02%	0.002%
76	9.697	2590	2599	2606	rVB3	1089	1730	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048518.D
 Acq On : 11 May 2022 15:42
 Operator : SY/MD
 Sample : N2790-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.989	2687	2690	2692	rVB2	262	146	0.01%	0.002%
78	10.050	2705	2709	2712	rBV	333	282	0.02%	0.003%
79	10.189	2750	2752	2756	rVB2	238	141	0.01%	0.002%
80	10.259	2771	2774	2775	rBV	234	142	0.01%	0.002%
81	10.308	2787	2789	2792	rBV	260	187	0.02%	0.002%
82	10.459	2832	2836	2840	rBV2	294	226	0.02%	0.002%
83	10.481	2840	2843	2847	rVB2	384	313	0.03%	0.003%
84	10.671	2895	2902	2909	rVB4	1691	2677	0.23%	0.029%
85	10.754	2916	2928	2944	rBV	396858	645650	54.31%	6.878%
86	10.867	2960	2963	2964	rBV	521	269	0.02%	0.003%
87	11.015	3006	3009	3010	rBV	225	133	0.01%	0.001%
88	11.095	3032	3034	3037	rBV	321	140	0.01%	0.001%
89	11.115	3037	3040	3044	rVV3	471	432	0.04%	0.005%
90	11.459	3141	3147	3158	rVB5	1979	2997	0.25%	0.032%
91	11.571	3179	3182	3186	rBV3	463	353	0.03%	0.004%
92	11.742	3233	3235	3239	rBV2	344	224	0.02%	0.002%
93	11.812	3244	3257	3275	rBV	542322	871381	73.30%	9.283%
94	12.192	3362	3375	3391	rBV	585134	936971	78.82%	9.982%
95	12.767	3550	3554	3560	rBV3	578	500	0.04%	0.005%
96	12.999	3623	3626	3629	rBV2	532	368	0.03%	0.004%
97	13.221	3693	3695	3698	rBV3	476	318	0.03%	0.003%
98	13.336	3728	3731	3734	rVB2	316	185	0.02%	0.002%
99	13.761	3860	3863	3867	rBV2	445	393	0.03%	0.004%
100	14.172	3988	3991	3998	rBV3	595	787	0.07%	0.008%




Sum of corrected areas: 9387026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048518.D
Acq On : 11 May 2022 15:42
Operator : SY/MD
Sample : N2790-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGNP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

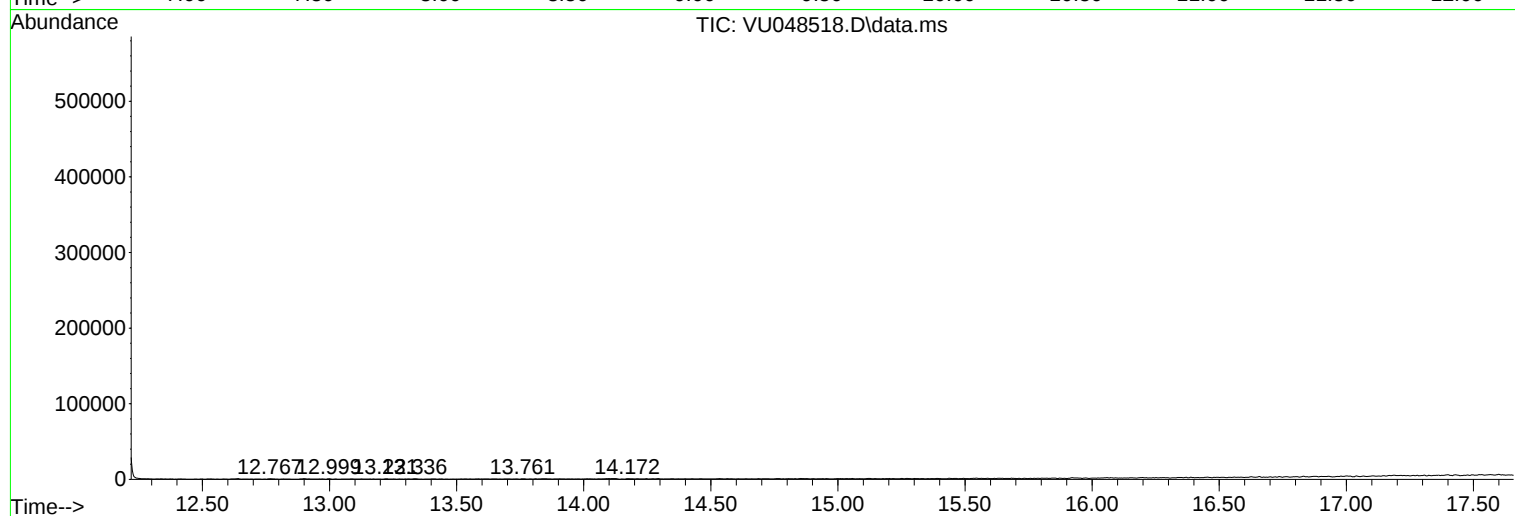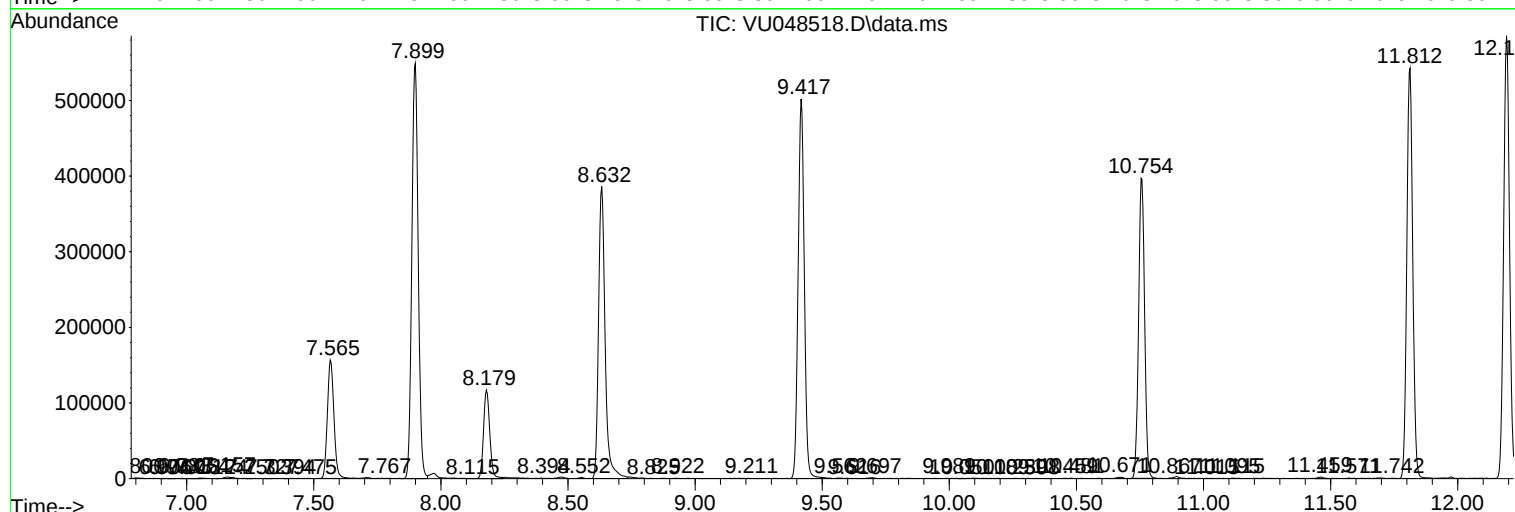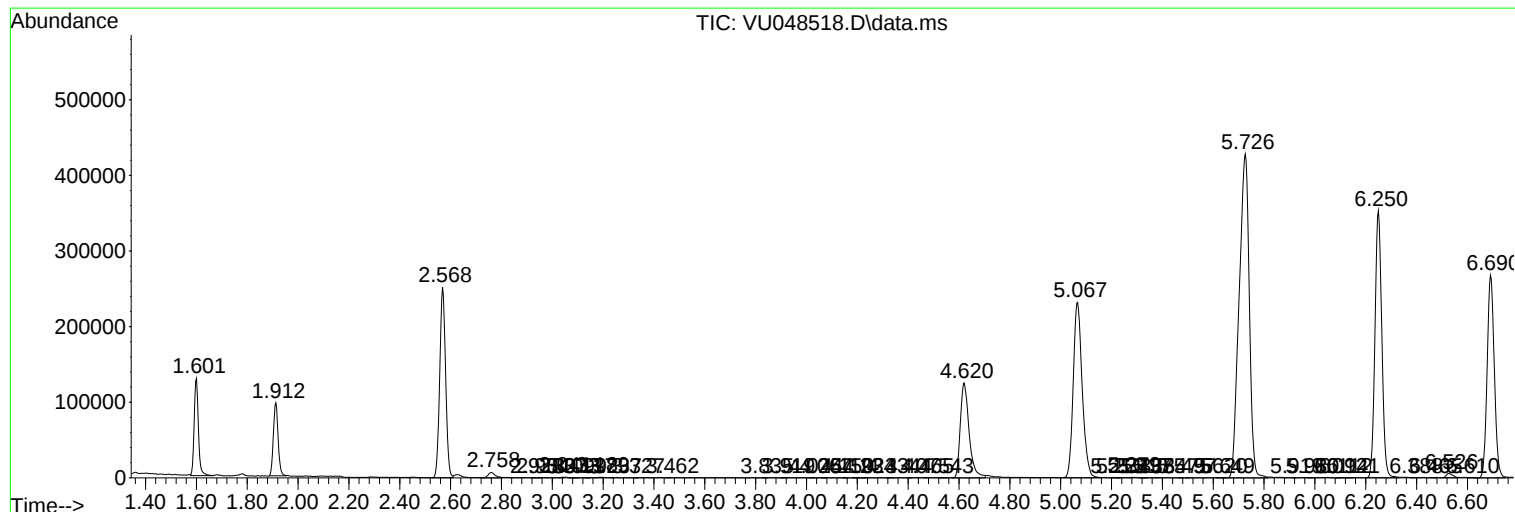

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048518.D
Acq On : 11 May 2022 15:42
Operator : SY/MD
Sample : N2790-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048518.D
Acq On : 11 May 2022 15:42
Operator : SY/MD
Sample : N2790-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc