

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048521.D
 Acq On : 11 May 2022 16:52
 Operator : SY/MD
 Sample : N2790-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rVB	123215	139404	12.96%	1.629%
2	1.912	170	178	198	rVB	91184	118725	11.04%	1.388%
3	2.568	369	382	394	rBV	219102	356129	33.12%	4.162%
4	2.771	434	445	462	rBV	6658	15385	1.43%	0.180%
5	2.854	465	471	472	rBV2	594	495	0.05%	0.006%
6	2.922	487	492	496	rBV2	359	440	0.04%	0.005%
7	2.961	502	504	507	rBV2	288	190	0.02%	0.002%
8	3.054	528	533	539	rBV4	566	596	0.06%	0.007%
9	3.276	598	602	603	rBV	270	206	0.02%	0.002%
10	3.334	617	620	625	rVV3	298	268	0.02%	0.003%
11	3.568	688	693	694	rBV2	381	305	0.03%	0.004%
12	3.645	713	717	721	rBB	198	177	0.02%	0.002%
13	3.668	722	724	729	rBV	347	382	0.04%	0.004%
14	3.700	731	734	738	rVB2	391	308	0.03%	0.004%
15	3.899	793	796	799	rBB	272	174	0.02%	0.002%
16	3.935	804	807	810	rVV	343	266	0.02%	0.003%
17	3.964	814	816	819	rVB2	374	206	0.02%	0.002%
18	3.993	820	825	828	rBB2	301	310	0.03%	0.004%
19	4.057	840	845	848	rBV	166	206	0.02%	0.002%
20	4.076	848	851	854	rVB	321	245	0.02%	0.003%
21	4.263	906	909	910	rBV	302	178	0.02%	0.002%
22	4.330	927	930	933	rVB	292	185	0.02%	0.002%
23	4.623	1005	1021	1044	rBV	105538	262516	24.41%	3.068%
24	5.067	1142	1159	1181	rBV	201393	444967	41.38%	5.200%
25	5.221	1203	1207	1212	rBV3	517	546	0.05%	0.006%
26	5.243	1212	1214	1216	rVB	427	202	0.02%	0.002%
27	5.260	1216	1219	1222	rBV	163	142	0.01%	0.002%
28	5.285	1224	1227	1228	rBV	605	344	0.03%	0.004%
29	5.324	1236	1239	1242	rVB	317	220	0.02%	0.003%
30	5.350	1243	1247	1251	rBV	351	378	0.04%	0.004%
31	5.378	1254	1256	1259	rBV	296	230	0.02%	0.003%
32	5.465	1277	1283	1286	rBB2	409	461	0.04%	0.005%
33	5.491	1288	1291	1295	rBV2	324	324	0.03%	0.004%
34	5.568	1307	1315	1317	rBV2	291	393	0.04%	0.005%
35	5.584	1317	1320	1324	rVB2	241	192	0.02%	0.002%
36	5.607	1324	1327	1330	rVB2	265	208	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048521.D
 Acq On : 11 May 2022 16:52
 Operator : SY/MD
 Sample : N2790-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.645	1337	1339	1341	rBV	310	177	0.02%	0.002%
38	5.726	1342	1364	1387	rBV2	393250	1075359	100.00%	12.568%
39	5.970	1438	1440	1447	rVB2	361	264	0.02%	0.003%
40	6.028	1454	1458	1460	rBV2	388	343	0.03%	0.004%
41	6.092	1476	1478	1480	rBV	273	152	0.01%	0.002%
42	6.163	1494	1500	1501	rBV2	448	451	0.04%	0.005%
43	6.250	1512	1527	1553	rBV	328030	625576	58.17%	7.311%
44	6.378	1564	1567	1569	rBV3	318	183	0.02%	0.002%
45	6.430	1579	1583	1586	rBV2	234	207	0.02%	0.002%
46	6.530	1605	1614	1632	rBV5	7879	16278	1.51%	0.190%
47	6.690	1650	1664	1682	rBV	244111	472040	43.90%	5.517%
48	6.890	1718	1726	1732	rBV5	1011	1668	0.16%	0.019%
49	6.951	1742	1745	1749	rBV2	343	372	0.03%	0.004%
50	6.980	1751	1754	1758	rVB2	364	298	0.03%	0.003%
51	7.012	1761	1764	1769	rVB	300	230	0.02%	0.003%
52	7.047	1770	1775	1776	rBV	346	273	0.03%	0.003%
53	7.150	1804	1807	1808	rBV2	302	204	0.02%	0.002%
54	7.179	1812	1816	1819	rVV3	633	588	0.05%	0.007%
55	7.195	1819	1821	1828	rVB3	419	361	0.03%	0.004%
56	7.304	1853	1855	1860	rVB2	404	260	0.02%	0.003%
57	7.433	1891	1895	1896	rBV	292	210	0.02%	0.002%
58	7.520	1918	1922	1923	rBV	265	183	0.02%	0.002%
59	7.568	1923	1937	1959	rVV	140996	251821	23.42%	2.943%
60	7.706	1978	1980	1986	rBV3	461	360	0.03%	0.004%
61	7.758	1993	1996	1999	rBV	330	287	0.03%	0.003%
62	7.787	1999	2005	2006	rBV2	406	409	0.04%	0.005%
63	7.899	2026	2040	2056	rBV	499377	855614	79.57%	9.999%
64	8.124	2108	2110	2116	rBV2	280	281	0.03%	0.003%
65	8.179	2116	2127	2146	rBV	104406	180107	16.75%	2.105%
66	8.475	2207	2219	2233	rVB3	4499	8476	0.79%	0.099%
67	8.549	2233	2242	2245	rBV4	976	1280	0.12%	0.015%
68	8.632	2255	2268	2298	rBV	342303	623661	58.00%	7.289%
69	8.829	2326	2329	2335	rVB5	696	635	0.06%	0.007%
70	8.896	2348	2350	2355	rBV	293	198	0.02%	0.002%
71	9.057	2397	2400	2404	rBV	366	340	0.03%	0.004%
72	9.243	2454	2458	2461	rBV2	275	234	0.02%	0.003%
73	9.279	2466	2469	2474	rBV	189	190	0.02%	0.002%
74	9.417	2498	2512	2533	rBV	478634	792735	73.72%	9.265%
75	9.574	2557	2561	2565	rVB3	813	629	0.06%	0.007%
76	9.600	2566	2569	2573	rVB2	390	257	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048521.D
 Acq On : 11 May 2022 16:52
 Operator : SY/MD
 Sample : N2790-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.745	2610	2614	2618	rVB2	215	189	0.02%	0.002%
78	9.851	2644	2647	2648	rBV	397	209	0.02%	0.002%
79	10.131	2731	2734	2738	rBV4	356	365	0.03%	0.004%
80	10.340	2796	2799	2802	rBV3	1088	908	0.08%	0.011%
81	10.674	2897	2903	2911	rVB4	1382	1708	0.16%	0.020%
82	10.758	2915	2929	2946	rBV	356238	580007	53.94%	6.778%
83	10.893	2964	2971	2981	rVB2	6296	8941	0.83%	0.104%
84	10.992	3000	3002	3004	rBV2	281	182	0.02%	0.002%
85	11.124	3036	3043	3046	rBV2	548	698	0.06%	0.008%
86	11.182	3058	3061	3068	rVB2	388	473	0.04%	0.006%
87	11.465	3138	3149	3161	rBV6	1564	2933	0.27%	0.034%
88	11.687	3212	3218	3228	rBV6	5343	8463	0.79%	0.099%
89	11.745	3233	3236	3241	rVB3	787	636	0.06%	0.007%
90	11.812	3244	3257	3275	rBV	521726	828041	77.00%	9.677%
91	12.073	3330	3338	3342	rBV5	957	1317	0.12%	0.015%
92	12.192	3362	3375	3392	rBV	528744	846259	78.70%	9.890%
93	12.513	3473	3475	3477	rBV	350	185	0.02%	0.002%
94	12.893	3584	3593	3605	rVB6	9118	14205	1.32%	0.166%
95	12.976	3617	3619	3628	rVB	387	394	0.04%	0.005%
96	13.012	3628	3630	3633	rBV	320	201	0.02%	0.002%
97	13.205	3686	3690	3693	rBV2	484	415	0.04%	0.005%
98	13.250	3701	3704	3710	rBV2	343	333	0.03%	0.004%
99	13.311	3721	3723	3725	rBV2	288	146	0.01%	0.002%
100	14.359	4046	4049	4051	rBV2	562	318	0.03%	0.004%




Sum of corrected areas: 8556620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048521.D
Acq On : 11 May 2022 16:52
Operator : SY/MD
Sample : N2790-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

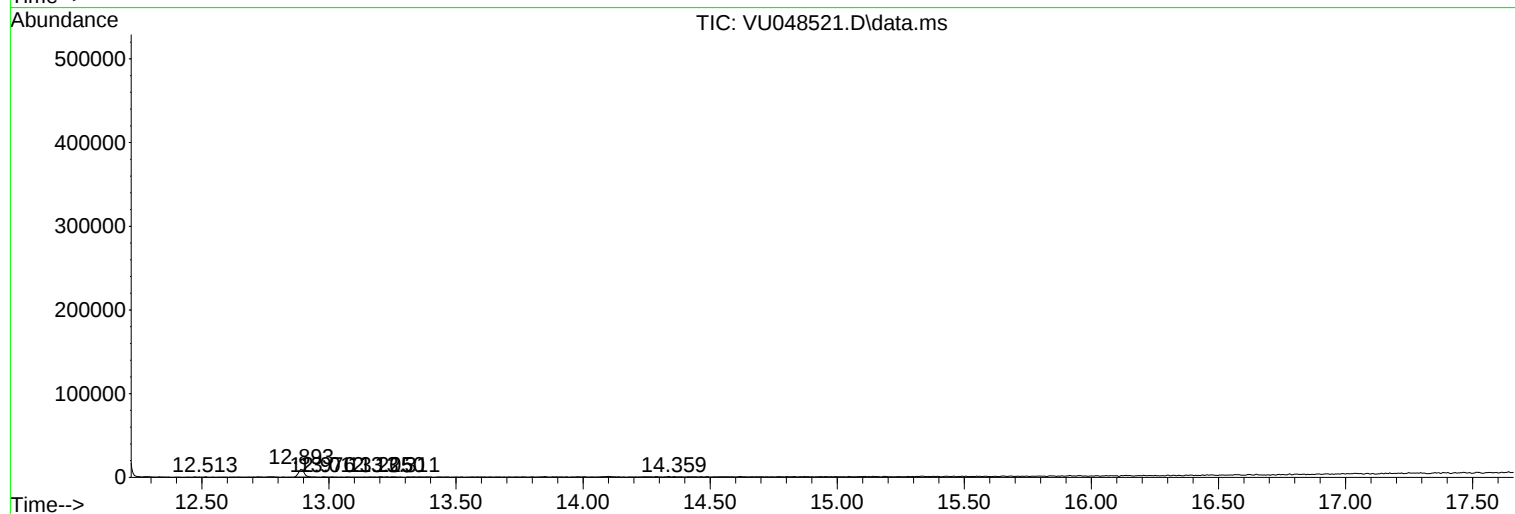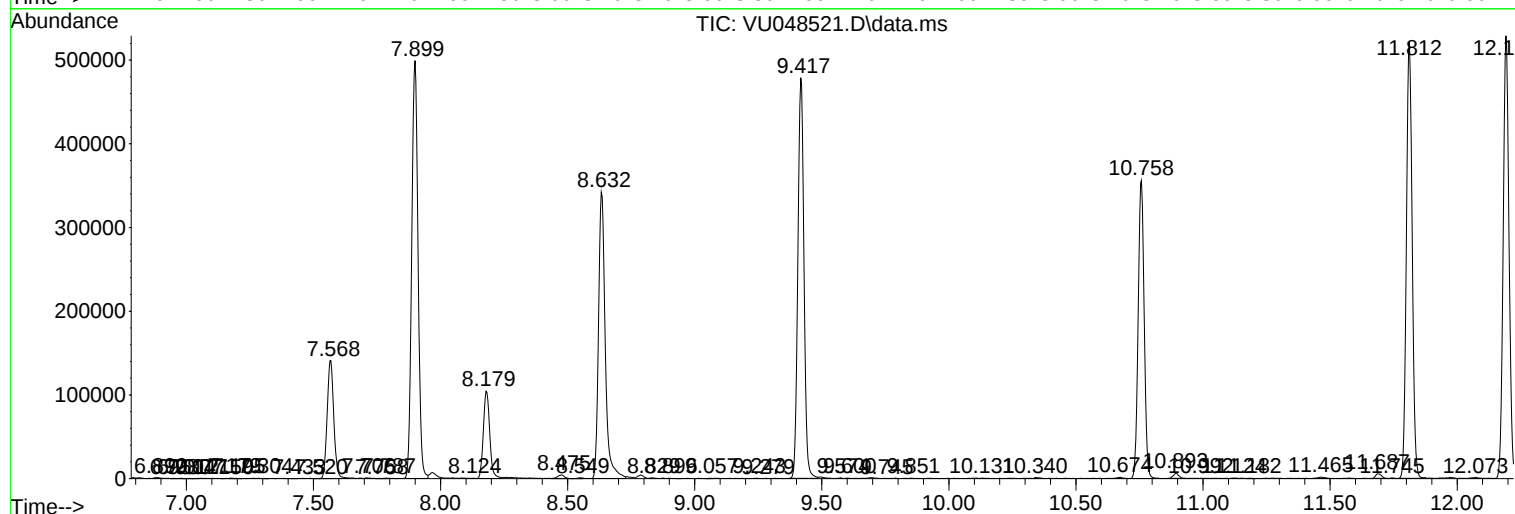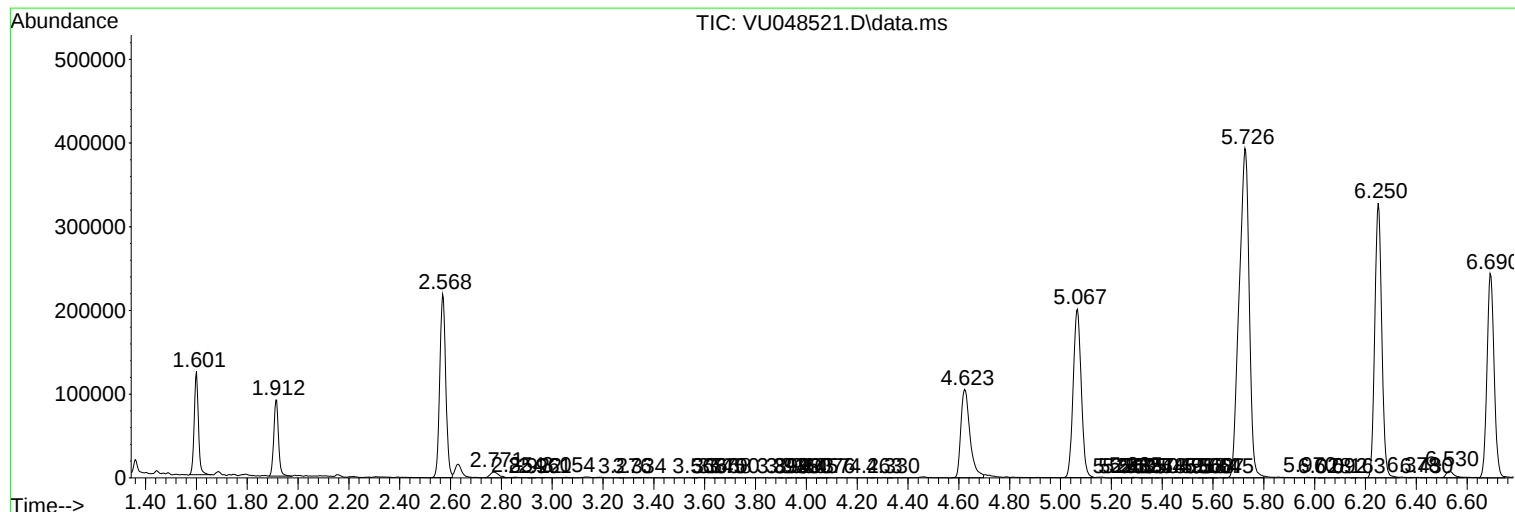

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048521.D
Acq On : 11 May 2022 16:52
Operator : SY/MD
Sample : N2790-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048521.D
Acq On : 11 May 2022 16:52
Operator : SY/MD
Sample : N2790-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------