

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048522.D
 Acq On : 11 May 2022 17:15
 Operator : SY/MD
 Sample : N2790-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	120155	138210	12.74%	1.591%
2	1.913	170	178	191	rBV	88582	114552	10.56%	1.319%
3	2.208	264	270	275	rBV5	1177	1597	0.15%	0.018%
4	2.408	325	332	335	rBV4	690	890	0.08%	0.010%
5	2.443	341	343	345	rBV	317	199	0.02%	0.002%
6	2.568	369	382	394	rBV	226425	367864	33.92%	4.235%
7	2.755	435	440	451	rVB3	2997	4520	0.42%	0.052%
8	2.861	467	473	476	rBV4	759	940	0.09%	0.011%
9	2.909	485	488	493	rVB2	269	242	0.02%	0.003%
10	3.048	528	531	535	rVB2	652	456	0.04%	0.005%
11	3.176	565	571	572	rBV	801	662	0.06%	0.008%
12	3.314	609	614	618	rVB3	502	514	0.05%	0.006%
13	3.395	636	639	643	rBV2	256	228	0.02%	0.003%
14	3.424	643	648	651	rBV2	294	296	0.03%	0.003%
15	3.572	689	694	695	rBV2	313	234	0.02%	0.003%
16	3.584	695	698	704	rVB4	647	672	0.06%	0.008%
17	3.636	709	714	719	rBV2	336	357	0.03%	0.004%
18	3.684	726	729	737	rVB2	320	351	0.03%	0.004%
19	3.726	738	742	747	rBV2	274	344	0.03%	0.004%
20	3.752	747	750	752	rBV	246	193	0.02%	0.002%
21	3.784	757	760	763	rBV	249	190	0.02%	0.002%
22	3.922	800	803	807	rVB2	397	237	0.02%	0.003%
23	3.951	808	812	815	rBB	223	198	0.02%	0.002%
24	4.035	835	838	843	rBV	194	221	0.02%	0.003%
25	4.221	891	896	899	rVB2	260	296	0.03%	0.003%
26	4.298	916	920	922	rBV	219	199	0.02%	0.002%
27	4.372	940	943	946	rVB	334	241	0.02%	0.003%
28	4.411	952	955	958	rBB2	271	187	0.02%	0.002%
29	4.456	958	969	971	rBV3	1181	1787	0.16%	0.021%
30	4.530	988	992	997	rVB2	388	370	0.03%	0.004%
31	4.559	997	1001	1002	rBV	328	209	0.02%	0.002%
32	4.620	1007	1020	1040	rBV	111496	262326	24.19%	3.020%
33	4.851	1090	1092	1096	rBV	335	219	0.02%	0.003%
34	4.938	1117	1119	1124	rVB2	443	257	0.02%	0.003%
35	4.967	1124	1128	1130	rBV2	300	210	0.02%	0.002%
36	5.064	1141	1158	1184	rBV	209981	479932	44.25%	5.525%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048522.D
 Acq On : 11 May 2022 17:15
 Operator : SY/MD
 Sample : N2790-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.231	1206	1210	1212	rBV2	451	343	0.03%	0.004%
38	5.285	1223	1227	1228	rBV	660	341	0.03%	0.004%
39	5.420	1265	1269	1275	rBV2	508	557	0.05%	0.006%
40	5.498	1289	1293	1295	rVB	295	209	0.02%	0.002%
41	5.523	1298	1301	1304	rBV	461	300	0.03%	0.003%
42	5.588	1319	1321	1325	rVB2	326	228	0.02%	0.003%
43	5.726	1339	1364	1393	rBV2	389845	1084562	100.00%	12.485%
44	5.903	1416	1419	1421	rBV2	458	268	0.02%	0.003%
45	5.919	1421	1424	1426	rBV	340	232	0.02%	0.003%
46	5.964	1433	1438	1441	rBV3	432	282	0.03%	0.003%
47	6.118	1482	1486	1488	rVB2	293	189	0.02%	0.002%
48	6.134	1488	1491	1493	rBV2	266	209	0.02%	0.002%
49	6.250	1512	1527	1546	rBV	342079	649792	59.91%	7.480%
50	6.424	1578	1581	1586	rVB3	476	413	0.04%	0.005%
51	6.446	1586	1588	1590	rBV2	394	229	0.02%	0.003%
52	6.530	1605	1614	1624	rBV6	4629	7656	0.71%	0.088%
53	6.690	1649	1664	1681	rBV	248434	480566	44.31%	5.532%
54	6.871	1717	1720	1721	rBV	385	189	0.02%	0.002%
55	6.890	1721	1726	1734	rVB4	800	1019	0.09%	0.012%
56	7.163	1804	1811	1821	rBV9	1562	2861	0.26%	0.033%
57	7.411	1886	1888	1895	rBV2	351	380	0.04%	0.004%
58	7.459	1898	1903	1907	rVV2	286	317	0.03%	0.004%
59	7.565	1924	1936	1955	rVV	142809	252183	23.25%	2.903%
60	7.780	1999	2003	2005	rBV	337	222	0.02%	0.003%
61	7.899	2026	2040	2055	rBV	496377	864302	79.69%	9.950%
62	8.179	2116	2127	2145	rBV	106136	179014	16.51%	2.061%
63	8.452	2205	2212	2213	rBV	737	609	0.06%	0.007%
64	8.478	2213	2220	2228	rVB3	2098	3485	0.32%	0.040%
65	8.555	2235	2244	2252	rBV4	6540	10199	0.94%	0.117%
66	8.633	2255	2268	2297	rBV	330236	612293	56.46%	7.049%
67	8.919	2354	2357	2360	rBV2	348	297	0.03%	0.003%
68	8.999	2379	2382	2384	rBV	327	252	0.02%	0.003%
69	9.070	2400	2404	2408	rBV2	320	339	0.03%	0.004%
70	9.192	2439	2442	2446	rVB2	478	339	0.03%	0.004%
71	9.417	2499	2512	2532	rBV	501218	820313	75.64%	9.443%
72	9.690	2586	2597	2599	rBV2	1128	1289	0.12%	0.015%
73	9.729	2606	2609	2612	rBV	201	198	0.02%	0.002%
74	9.883	2655	2657	2662	rVB2	255	200	0.02%	0.002%
75	10.346	2797	2801	2807	rBV3	960	1072	0.10%	0.012%
76	10.436	2827	2829	2833	rVB	311	204	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048522.D
 Acq On : 11 May 2022 17:15
 Operator : SY/MD
 Sample : N2790-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.616	2883	2885	2891	rVB2	589	455	0.04%	0.005%
78	10.645	2891	2894	2896	rBV2	279	196	0.02%	0.002%
79	10.668	2896	2901	2913	rVV4	2125	2411	0.22%	0.028%
80	10.758	2916	2929	2948	rVB	358803	585004	53.94%	6.734%
81	10.867	2959	2963	2964	rBV	433	250	0.02%	0.003%
82	10.893	2964	2971	2987	rVB6	3137	5319	0.49%	0.061%
83	11.002	3003	3005	3010	rBV3	325	278	0.03%	0.003%
84	11.047	3017	3019	3023	rVB2	703	335	0.03%	0.004%
85	11.086	3029	3031	3036	rVB2	329	198	0.02%	0.002%
86	11.465	3140	3149	3156	rBV6	1325	2463	0.23%	0.028%
87	11.613	3193	3195	3201	rVV	400	342	0.03%	0.004%
88	11.645	3201	3205	3207	rVB	511	300	0.03%	0.003%
89	11.693	3212	3220	3233	rBV6	6930	12094	1.12%	0.139%
90	11.812	3245	3257	3276	rVV	534985	844067	77.83%	9.717%
91	11.912	3286	3288	3289	rBV	407	191	0.02%	0.002%
92	12.192	3362	3375	3393	rVV	523536	857099	79.03%	9.867%
93	12.304	3408	3410	3413	rBV2	448	296	0.03%	0.003%
94	12.864	3580	3584	3585	rBV	297	202	0.02%	0.002%
95	12.893	3585	3593	3603	rVB5	10062	15718	1.45%	0.181%
96	13.269	3707	3710	3714	rVB2	422	225	0.02%	0.003%
97	13.372	3739	3742	3743	rBV	577	317	0.03%	0.004%
98	13.475	3771	3774	3778	rBV	356	193	0.02%	0.002%
99	13.771	3863	3866	3869	rBV	275	225	0.02%	0.003%
100	14.253	4013	4016	4017	rBV	368	187	0.02%	0.002%




Sum of corrected areas: 8686717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048522.D
Acq On : 11 May 2022 17:15
Operator : SY/MD
Sample : N2790-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGNP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

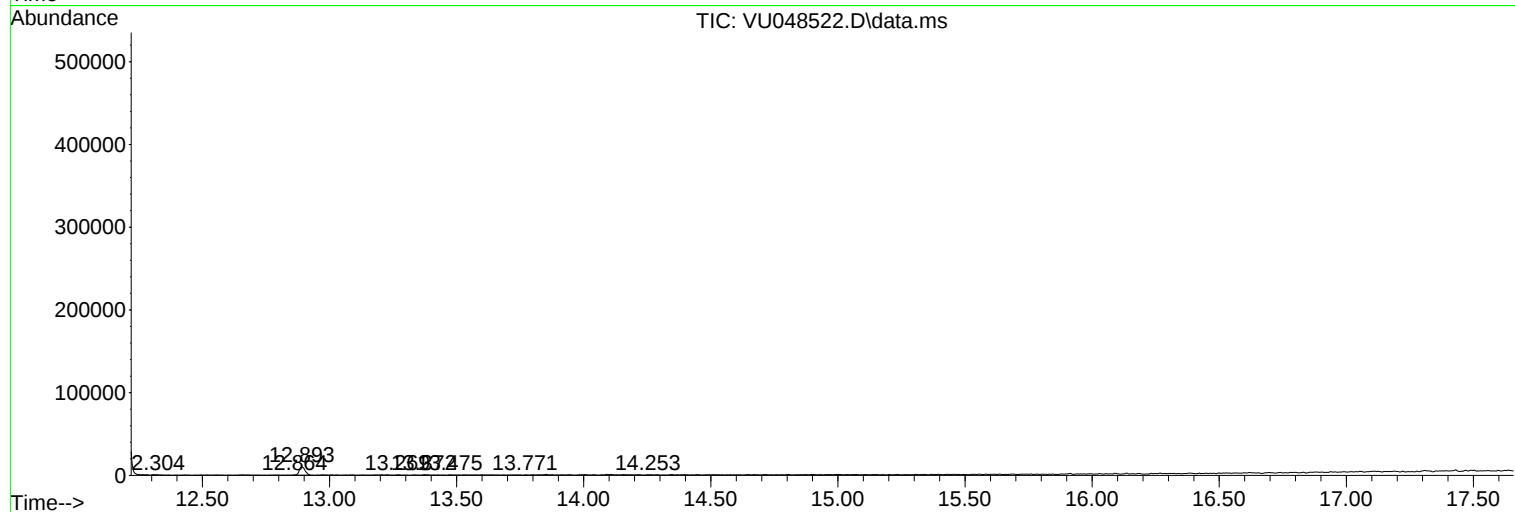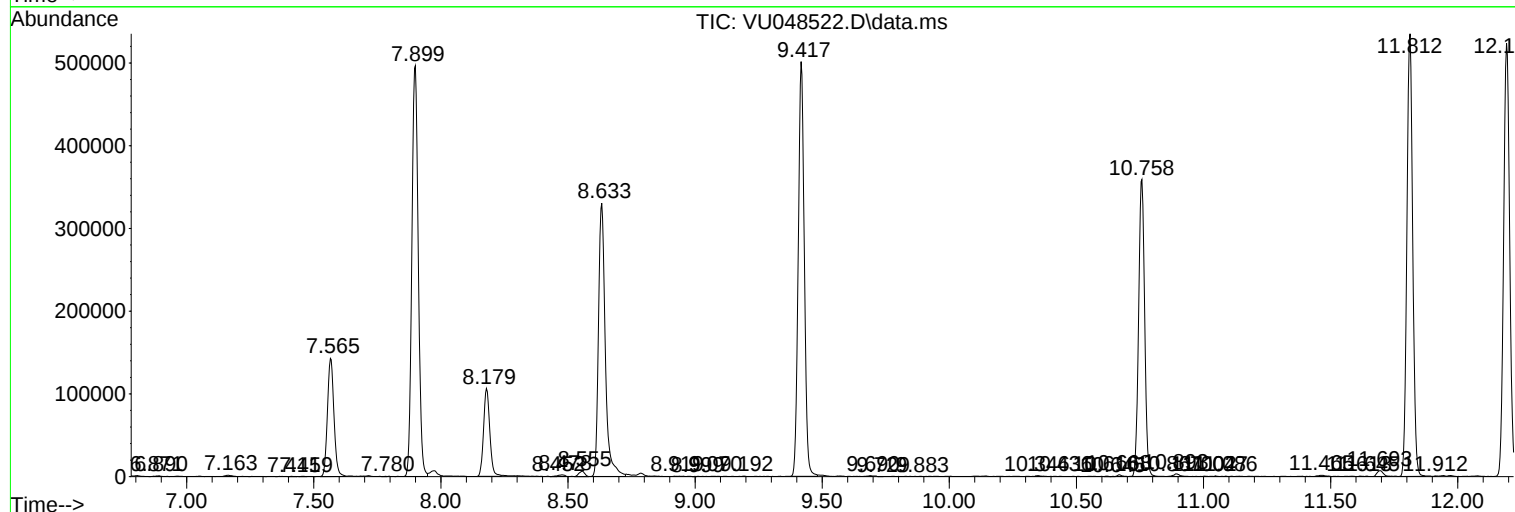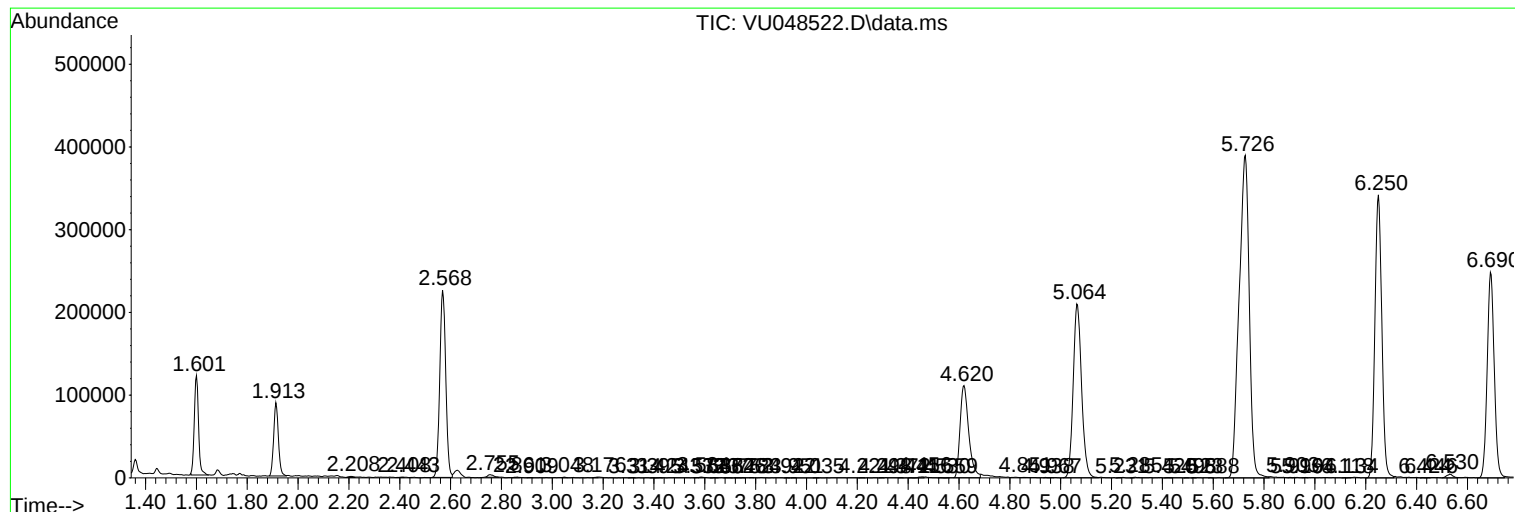

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048522.D
Acq On : 11 May 2022 17:15
Operator : SY/MD
Sample : N2790-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048522.D
Acq On : 11 May 2022 17:15
Operator : SY/MD
Sample : N2790-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------