

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048525.D
 Acq On : 11 May 2022 18:25
 Operator : SY/MD
 Sample : N2790-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	96	rVB	109323	125451	11.63%	1.446%
2	1.912	170	178	194	rVB	88410	113967	10.56%	1.313%
3	2.314	301	303	310	rVB3	521	391	0.04%	0.005%
4	2.568	370	382	396	rBV	219486	360668	33.42%	4.156%
5	2.768	434	444	456	rBV2	3629	7228	0.67%	0.083%
6	2.867	473	475	480	rBV2	271	227	0.02%	0.003%
7	3.038	525	528	530	rBV2	239	194	0.02%	0.002%
8	3.298	603	609	612	rBB2	410	401	0.04%	0.005%
9	3.324	613	617	623	rBV2	275	392	0.04%	0.005%
10	3.375	627	633	639	rVB3	537	791	0.07%	0.009%
11	3.404	640	642	647	rBV	297	276	0.03%	0.003%
12	3.443	650	654	656	rBV2	327	297	0.03%	0.003%
13	3.494	665	670	673	rVB2	385	376	0.03%	0.004%
14	3.517	674	677	679	rBV	213	172	0.02%	0.002%
15	3.739	744	746	750	rBV	239	183	0.02%	0.002%
16	3.922	799	803	806	rBV	342	326	0.03%	0.004%
17	3.967	812	817	824	rBB2	327	490	0.05%	0.006%
18	4.018	830	833	836	rBV	172	177	0.02%	0.002%
19	4.060	843	846	849	rBV	193	183	0.02%	0.002%
20	4.083	849	853	856	rVV	217	168	0.02%	0.002%
21	4.182	882	884	886	rBV	271	161	0.01%	0.002%
22	4.295	914	919	921	rBV	330	261	0.02%	0.003%
23	4.311	922	924	930	rVB2	418	317	0.03%	0.004%
24	4.343	930	934	939	rBB2	285	272	0.03%	0.003%
25	4.372	939	943	945	rBV2	293	216	0.02%	0.002%
26	4.488	974	979	983	rBB2	313	364	0.03%	0.004%
27	4.543	992	996	997	rBV	260	195	0.02%	0.002%
28	4.620	1008	1020	1048	rBV	108474	274382	25.43%	3.162%
29	5.063	1142	1158	1182	rBV	207330	461783	42.79%	5.321%
30	5.205	1199	1202	1205	rBV2	361	270	0.03%	0.003%
31	5.221	1205	1207	1210	rVB2	382	222	0.02%	0.003%
32	5.266	1217	1221	1225	rBV	240	314	0.03%	0.004%
33	5.288	1225	1228	1234	rVB2	577	526	0.05%	0.006%
34	5.324	1236	1239	1241	rVB2	269	167	0.02%	0.002%
35	5.343	1242	1245	1248	rBV	178	185	0.02%	0.002%
36	5.362	1249	1251	1254	rBV2	270	164	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048525.D
 Acq On : 11 May 2022 18:25
 Operator : SY/MD
 Sample : N2790-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.395	1259	1261	1265	rBV2	384	324	0.03%	0.004%
38	5.440	1272	1275	1277	rVB2	454	247	0.02%	0.003%
39	5.465	1277	1283	1285	rBV	188	234	0.02%	0.003%
40	5.539	1302	1306	1310	rBV	281	266	0.02%	0.003%
41	5.578	1314	1318	1321	rBV2	262	220	0.02%	0.003%
42	5.626	1329	1333	1337	rBV	202	180	0.02%	0.002%
43	5.726	1343	1364	1393	rBV2	386939	1079100	100.00%	12.434%
44	5.941	1429	1431	1435	rVB2	369	205	0.02%	0.002%
45	6.250	1510	1527	1548	rBV	347793	661776	61.33%	7.625%
46	6.526	1606	1613	1628	rVB6	5831	10240	0.95%	0.118%
47	6.690	1648	1664	1685	rBV	247750	482930	44.75%	5.565%
48	6.780	1689	1692	1694	rBV2	389	177	0.02%	0.002%
49	6.841	1708	1711	1715	rBV2	216	193	0.02%	0.002%
50	6.883	1719	1724	1727	rBV	456	303	0.03%	0.003%
51	6.999	1757	1760	1764	rBV2	316	261	0.02%	0.003%
52	7.144	1803	1805	1809	rBV2	276	200	0.02%	0.002%
53	7.163	1809	1811	1813	rBV2	565	346	0.03%	0.004%
54	7.259	1838	1841	1843	rBV	245	164	0.02%	0.002%
55	7.311	1854	1857	1862	rBV2	328	388	0.04%	0.004%
56	7.366	1868	1874	1877	rBV	278	338	0.03%	0.004%
57	7.385	1877	1880	1883	rVB	389	271	0.03%	0.003%
58	7.565	1924	1936	1955	rBV	142299	249683	23.14%	2.877%
59	7.677	1965	1971	1972	rBV2	566	501	0.05%	0.006%
60	7.742	1987	1991	1992	rBV	451	199	0.02%	0.002%
61	7.812	2009	2013	2018	rBV	346	341	0.03%	0.004%
62	7.899	2026	2040	2057	rBV	503213	865976	80.25%	9.978%
63	8.179	2115	2127	2150	rBV	105768	180381	16.72%	2.078%
64	8.417	2199	2201	2206	rVB	347	171	0.02%	0.002%
65	8.446	2206	2210	2211	rBV2	291	178	0.02%	0.002%
66	8.468	2211	2217	2219	rBV2	1322	1476	0.14%	0.017%
67	8.578	2249	2251	2255	rVB	387	234	0.02%	0.003%
68	8.632	2256	2268	2302	rBV	360249	647328	59.99%	7.459%
69	8.915	2352	2356	2359	rBV	233	203	0.02%	0.002%
70	9.009	2383	2385	2391	rVB2	328	244	0.02%	0.003%
71	9.163	2431	2433	2439	rVB	361	279	0.03%	0.003%
72	9.227	2449	2453	2456	rBV	219	160	0.01%	0.002%
73	9.417	2499	2512	2535	rBV	499488	829537	76.87%	9.559%
74	9.648	2581	2584	2592	rVV2	341	457	0.04%	0.005%
75	9.693	2592	2598	2606	rVB3	895	1201	0.11%	0.014%
76	9.941	2673	2675	2679	rBV	426	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048525.D
 Acq On : 11 May 2022 18:25
 Operator : SY/MD
 Sample : N2790-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.092	2720	2722	2725	rBV	370	221	0.02%	0.003%
78	10.189	2746	2752	2753	rBV2	309	319	0.03%	0.004%
79	10.671	2894	2902	2903	rBV3	1442	1426	0.13%	0.016%
80	10.754	2916	2928	2945	rBV	354270	584686	54.18%	6.737%
81	10.896	2962	2972	2978	rBV2	2138	3242	0.30%	0.037%
82	11.140	3046	3048	3051	rBV2	319	187	0.02%	0.002%
83	11.362	3113	3117	3120	rBV	307	232	0.02%	0.003%
84	11.446	3139	3143	3145	rBV3	893	674	0.06%	0.008%
85	11.661	3207	3210	3211	rBV2	288	170	0.02%	0.002%
86	11.735	3231	3233	3236	rBV	331	165	0.02%	0.002%
87	11.748	3236	3237	3241	rVB	493	215	0.02%	0.002%
88	11.812	3244	3257	3282	rBV	541646	854680	79.20%	9.848%
89	12.115	3346	3351	3352	rBV	331	252	0.02%	0.003%
90	12.192	3361	3375	3393	rBV	523964	859287	79.63%	9.901%
91	12.275	3398	3401	3403	rVB2	738	344	0.03%	0.004%
92	12.343	3416	3422	3427	rBV4	649	798	0.07%	0.009%
93	12.774	3553	3556	3557	rBV4	329	183	0.02%	0.002%
94	12.957	3610	3613	3616	rBV2	332	266	0.02%	0.003%
95	13.153	3668	3674	3677	rBV3	423	466	0.04%	0.005%
96	13.571	3802	3804	3806	rBV	359	169	0.02%	0.002%
97	13.619	3818	3819	3824	rVB	381	230	0.02%	0.003%
98	13.645	3824	3827	3829	rBV	364	232	0.02%	0.003%
99	13.761	3860	3863	3865	rBV	482	309	0.03%	0.004%
100	13.803	3873	3876	3879	rBV	501	439	0.04%	0.005%




Sum of corrected areas: 8678514

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048525.D
Acq On : 11 May 2022 18:25
Operator : SY/MD
Sample : N2790-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPNO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

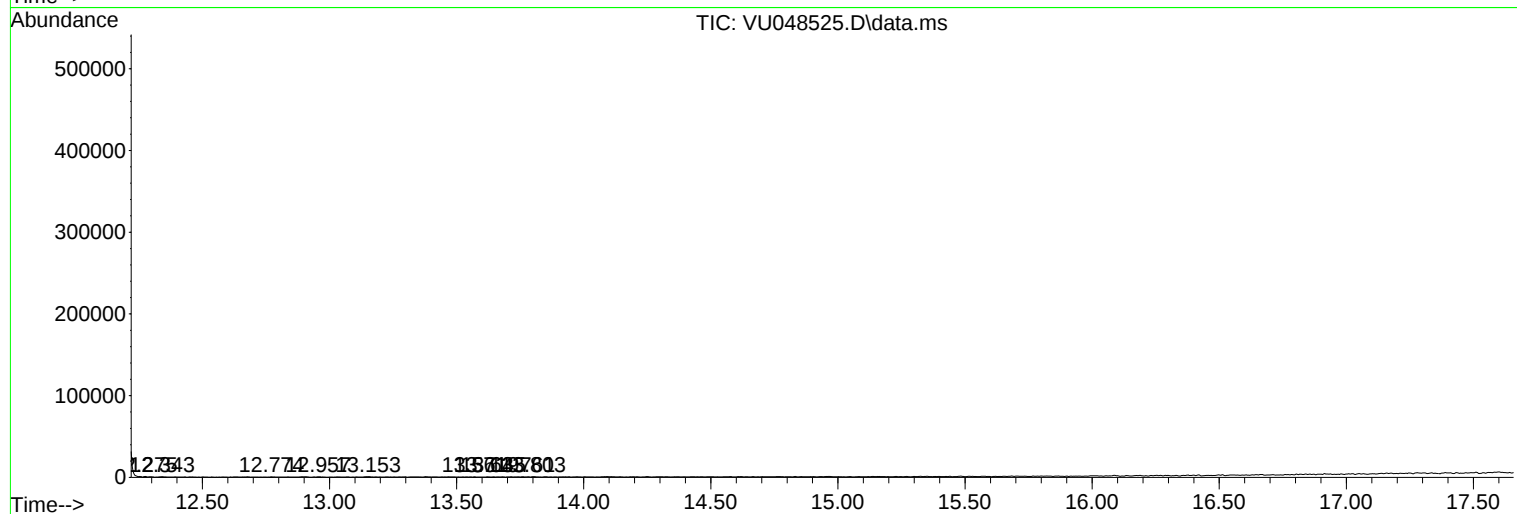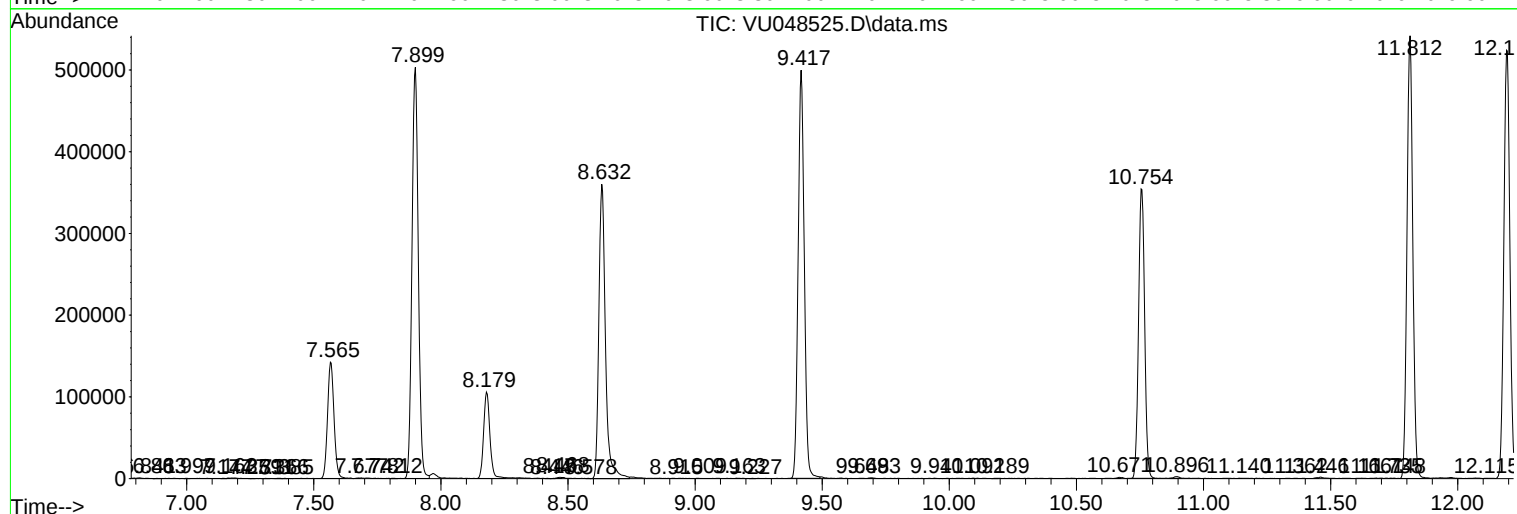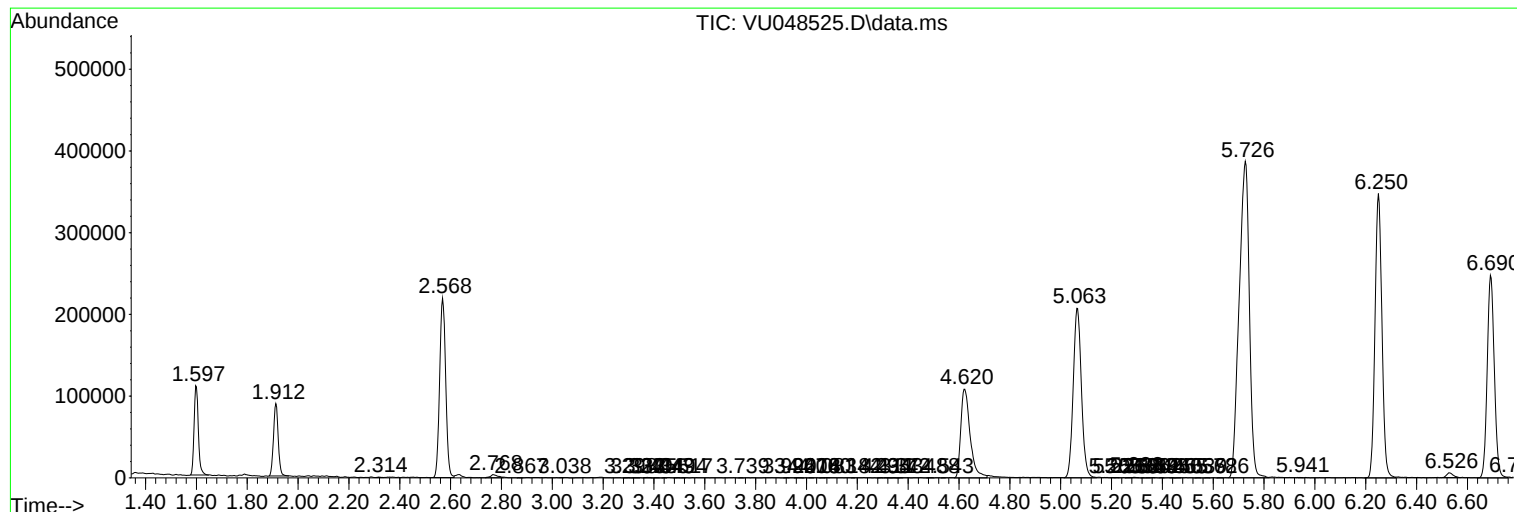

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048525.D
Acq On : 11 May 2022 18:25
Operator : SY/MD
Sample : N2790-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPNO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
Data File : VU048525.D
Acq On : 11 May 2022 18:25
Operator : SY/MD
Sample : N2790-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPNO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc