
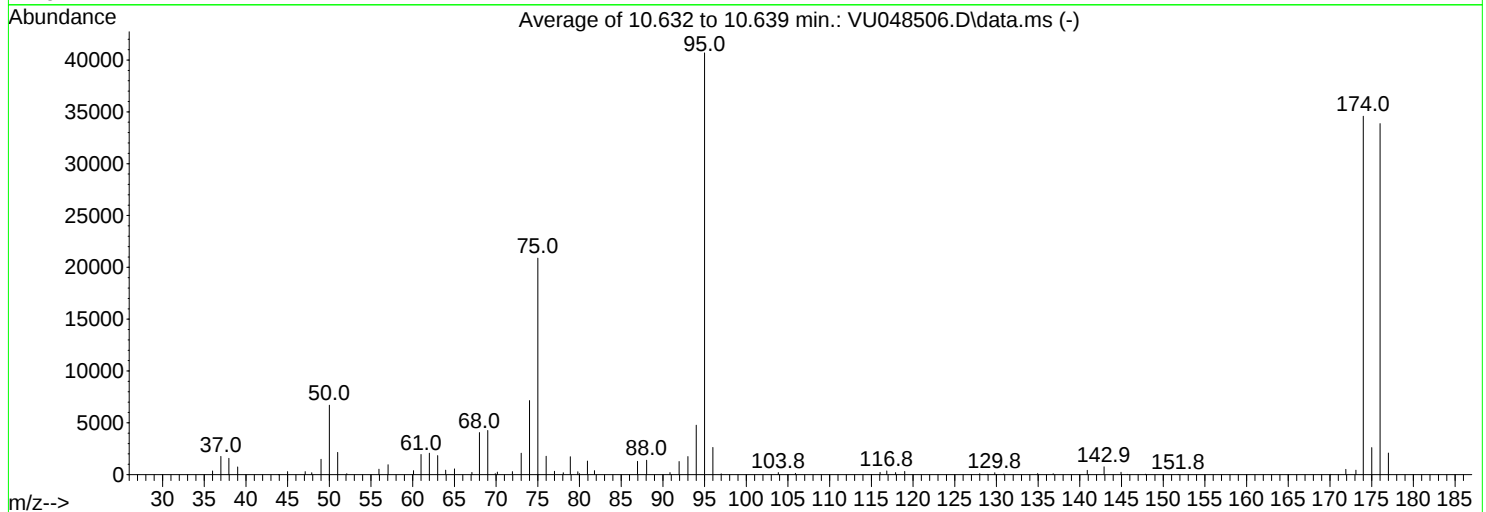


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051122\
 Data File : VU048506.D
 Acq On : 11 May 2022 10:09
 Operator : SY/MD
 Sample : BFB083
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB083

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis
 Last Update : Fri May 13 03:54:05 2022

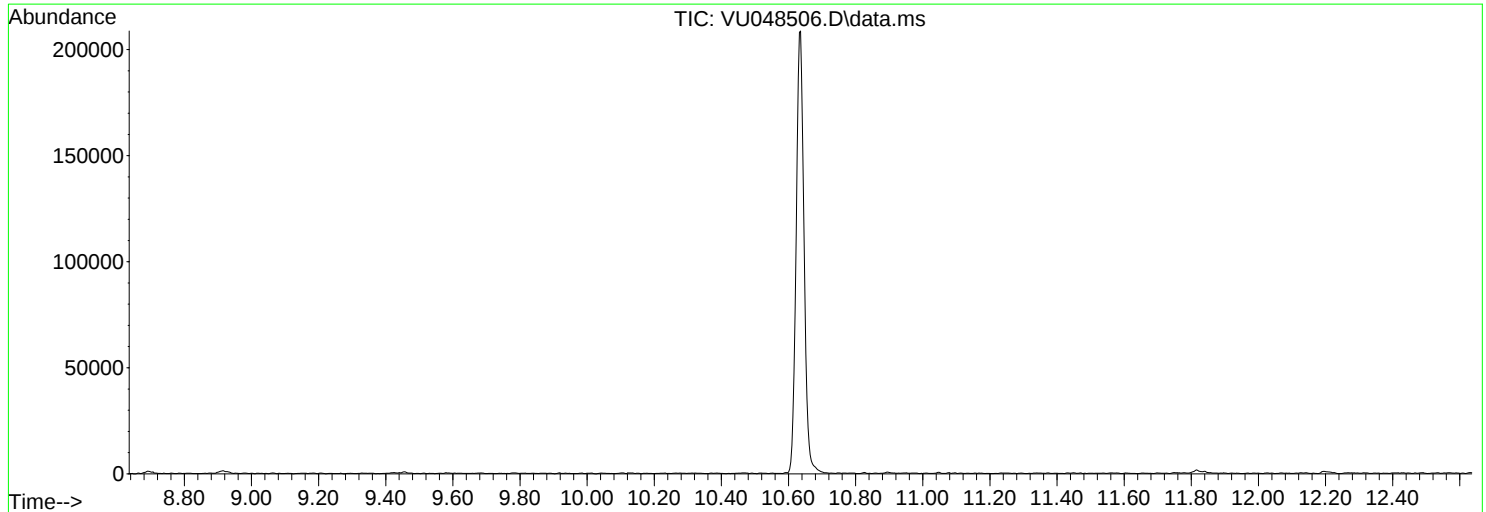

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	6695	PASS
75	95	30	80	51.3	20883	PASS
95	95	100	100	100.0	40693	PASS
96	95	5	9	6.4	2619	PASS
173	174	0.00	2	1.3	439	PASS
174	95	50	120	85.0	34573	PASS
175	174	5	9	7.5	2610	PASS
176	174	95	101	98.0	33875	PASS
177	176	5	9	6.2	2093	PASS

m/z	Abundance
36.00	323.0
37.00	1565.0
37.90	1376.0
39.00	673.0
39.70	143.0
44.00	419.0
45.00	266.0
47.10	265.0
47.80	133.0
49.00	1342.0
50.00	6118.0
51.00	2096.0
52.10	148.0
56.00	515.0
57.10	760.0
60.10	348.0
61.00	1773.0
62.00	1787.0
63.00	1826.0
64.00	393.0
65.00	529.0
67.10	285.0
68.00	3624.0
69.00	3808.0
69.90	298.0
71.90	297.0
73.00	1957.0
74.00	6442.0
75.00	19624.0
76.00	1632.0
77.00	297.0
78.00	130.0
78.90	1661.0
79.80	275.0
81.00	1223.0
81.80	364.0
87.00	1224.0
88.10	1121.0
90.80	157.0
91.90	1139.0
93.00	1723.0
94.00	4308.0
95.00	38344.0
96.00	2260.0
103.80	198.0
105.90	111.0
116.10	228.0
116.80	332.0
118.00	177.0
119.00	303.0
129.80	212.0
135.00	108.0
136.80	151.0
140.90	410.0
142.90	693.0
144.90	219.0
145.70	100.0
147.90	125.0
170.10	105.0
171.80	474.0
174.00	32872.0
175.00	2398.0
176.00	32600.0
177.00	1955.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
39.90	241.0
43.90	368.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
36.00	401.0
37.00	1869.0
38.00	1754.0
39.00	773.0
43.90	318.0
45.00	323.0
47.10	309.0
48.00	240.0
49.00	1606.0
50.00	7108.0
51.00	2147.0
55.90	524.0
57.00	1153.0
60.10	438.0
61.00	2108.0
62.00	2270.0
63.00	1826.0
63.90	425.0
65.00	583.0
67.10	152.0
68.00	4362.0
69.00	4552.0
70.20	394.0
72.10	270.0
73.00	2119.0
74.00	7612.0
75.00	21640.0
76.00	1861.0
77.00	332.0
78.10	237.0
78.90	1667.0
79.80	297.0
80.90	1401.0
81.80	383.0
86.90	1297.0
88.00	1642.0
90.90	231.0
92.00	1364.0
93.00	1742.0
94.00	5152.0
95.00	41608.0
96.00	2880.0
97.00	133.0
103.90	214.0
105.90	133.0
116.00	197.0
116.90	359.0
117.80	233.0
119.00	293.0
128.00	151.0
129.80	169.0
130.90	100.0
134.90	101.0
140.90	444.0
142.90	784.0
145.00	231.0
151.80	114.0
172.00	537.0
173.10	658.0
174.00	35048.0
175.00	2770.0
176.00	33912.0
177.00	2167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
36.00	352.0
37.00	1840.0
38.00	1608.0
39.00	775.0
44.00	389.0
45.00	300.0
47.10	307.0
47.80	167.0
49.00	1513.0
50.00	6858.0
51.00	2177.0
52.10	151.0
55.90	551.0
57.10	974.0
60.10	394.0
61.00	1964.0
62.00	2133.0
63.00	1880.0
64.00	460.0
65.00	569.0
67.10	226.0
68.00	4213.0
69.00	4408.0
70.10	350.0
71.90	320.0
73.00	2135.0
74.00	7381.0
75.00	21384.0
76.00	1832.0
77.00	341.0
78.00	191.0
78.90	1847.0
79.80	266.0
80.00	268.0
80.90	1317.0
81.80	411.0
86.90	1330.0
88.00	1415.0
90.90	214.0
92.00	1280.0
93.00	1785.0
94.00	4860.0
95.00	42128.0
96.00	2716.0
97.00	107.0
103.90	198.0
105.90	126.0
116.10	244.0
116.80	374.0
117.90	209.0
119.00	328.0
128.00	145.0
128.90	100.0
129.80	183.0
130.90	101.0
134.90	132.0
136.80	132.0
140.90	414.0
142.90	803.0
145.00	240.0
171.90	520.0
173.10	659.0
174.00	35800.0
175.00	2661.0
176.00	35112.0
177.00	2156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083