

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
 Data File : VU054152.D
 Acq On : 11 May 2023 11:05
 Operator : JC/MD
 Sample : VU0511WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK095

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rVB	94494	115662	13.49%	1.729%
2	1.909	170	177	194	rVB	73020	102099	11.90%	1.526%
3	2.565	369	381	400	rBV	167319	273493	31.89%	4.089%
4	2.790	442	451	456	rBV3	420	728	0.08%	0.011%
5	2.884	478	480	481	rBV3	144	46	0.01%	0.001%
6	3.006	517	518	521	rBV	210	102	0.01%	0.002%
7	3.048	521	531	540	rVV4	3385	6698	0.78%	0.100%
8	3.131	554	557	564	rVB2	245	215	0.03%	0.003%
9	3.163	564	567	569	rBV	221	115	0.01%	0.002%
10	3.311	611	613	615	rVB	275	79	0.01%	0.001%
11	3.331	615	619	623	rBV2	377	297	0.03%	0.004%
12	3.459	654	659	661	rBV	185	169	0.02%	0.003%
13	3.495	668	670	673	rBV	203	128	0.01%	0.002%
14	3.887	789	792	795	rVB	224	115	0.01%	0.002%
15	3.980	819	821	823	rBV	139	52	0.01%	0.001%
16	4.009	827	830	840	rVB	271	254	0.03%	0.004%
17	4.118	862	864	871	rVB	224	142	0.02%	0.002%
18	4.176	879	882	888	rVB	201	134	0.02%	0.002%
19	4.308	920	923	925	rBV	158	67	0.01%	0.001%
20	4.620	1008	1020	1044	rBV	63350	161884	18.88%	2.420%
21	5.057	1132	1156	1183	rBV	159692	357799	41.72%	5.349%
22	5.273	1221	1223	1224	rVB	129	30	0.00%	0.000%
23	5.363	1249	1251	1253	rBV	149	40	0.00%	0.001%
24	5.501	1291	1294	1297	rBV	123	75	0.01%	0.001%
25	5.514	1297	1298	1300	rBV	111	45	0.01%	0.001%
26	5.601	1320	1325	1330	rBV	354	431	0.05%	0.006%
27	5.720	1341	1362	1382	rBV2	311646	857615	100.00%	12.821%
28	5.974	1439	1441	1443	rBV	344	210	0.02%	0.003%
29	6.015	1451	1454	1456	rBV2	329	226	0.03%	0.003%
30	6.064	1463	1469	1471	rBV2	342	283	0.03%	0.004%
31	6.102	1476	1481	1485	rVB	105	92	0.01%	0.001%
32	6.125	1485	1488	1492	rBV2	208	138	0.02%	0.002%
33	6.147	1493	1495	1499	rVB	218	148	0.02%	0.002%
34	6.244	1510	1525	1547	rBV	292764	558395	65.11%	8.348%
35	6.504	1603	1606	1607	rBV	685	317	0.04%	0.005%
36	6.527	1607	1613	1615	rBV5	1723	2021	0.24%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
 Data File : VU054152.D
 Acq On : 11 May 2023 11:05
 Operator : JC/MD
 Sample : VU0511WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK095

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.636	1645	1647	1649	rBV	137	40	0.00%	0.001%
38	6.684	1649	1662	1685	rBV	199188	393704	45.91%	5.886%
39	6.912	1729	1733	1735	rBV	142	115	0.01%	0.002%
40	6.964	1746	1749	1751	rBV	178	139	0.02%	0.002%
41	7.019	1764	1766	1770	rBV	171	126	0.01%	0.002%
42	7.205	1816	1824	1829	rVB2	419	599	0.07%	0.009%
43	7.276	1842	1846	1847	rBV	166	110	0.01%	0.002%
44	7.298	1852	1853	1854	rBV	117	28	0.00%	0.000%
45	7.562	1922	1935	1955	rBV2	112577	202011	23.55%	3.020%
46	7.684	1971	1973	1975	rBV	290	180	0.02%	0.003%
47	7.710	1978	1981	1985	rVB2	371	266	0.03%	0.004%
48	7.845	2020	2023	2024	rBV	138	76	0.01%	0.001%
49	7.893	2024	2038	2076	rVV	392552	683080	79.65%	10.212%
50	8.176	2115	2126	2142	rBV	81376	137638	16.05%	2.058%
51	8.276	2155	2157	2160	rVB	263	109	0.01%	0.002%
52	8.311	2165	2168	2171	rBV	244	186	0.02%	0.003%
53	8.398	2193	2195	2197	rBV	358	174	0.02%	0.003%
54	8.449	2209	2211	2214	rBV	232	109	0.01%	0.002%
55	8.543	2237	2240	2241	rBV	258	119	0.01%	0.002%
56	8.629	2256	2267	2302	rBV2	188367	371616	43.33%	5.555%
57	8.829	2325	2329	2333	rBV3	362	305	0.04%	0.005%
58	8.899	2348	2351	2353	rBV	156	88	0.01%	0.001%
59	8.935	2359	2362	2363	rBV	190	90	0.01%	0.001%
60	9.144	2425	2427	2428	rBV	146	57	0.01%	0.001%
61	9.231	2451	2454	2456	rBV	266	195	0.02%	0.003%
62	9.327	2481	2484	2486	rBV	202	95	0.01%	0.001%
63	9.411	2498	2510	2531	rBV	403326	672551	78.42%	10.054%
64	9.645	2582	2583	2584	rBV	244	60	0.01%	0.001%
65	10.025	2699	2701	2704	rVB2	193	108	0.01%	0.002%
66	10.115	2727	2729	2732	rBV	403	233	0.03%	0.003%
67	10.182	2748	2750	2754	rVB	262	159	0.02%	0.002%
68	10.202	2754	2756	2757	rBV	194	87	0.01%	0.001%
69	10.752	2915	2927	2941	rBV	277522	440332	51.34%	6.583%
70	11.253	3081	3083	3085	rBV	182	85	0.01%	0.001%
71	11.266	3085	3087	3090	rVV	178	77	0.01%	0.001%
72	11.716	3224	3227	3229	rBV	261	154	0.02%	0.002%
73	11.806	3243	3255	3276	rBV	415928	663449	77.36%	9.918%
74	12.189	3361	3374	3399	rBV	414742	677437	78.99%	10.127%
75	12.960	3611	3614	3617	rBV	407	369	0.04%	0.006%
76	13.231	3691	3698	3703	rBV3	791	1151	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
Data File : VU054152.D
Acq On : 11 May 2023 11:05
Operator : JC/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK095

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis

77	13.845	3886	3889	3897	rVB3	1459	1388	0.16%	0.021%
----	--------	------	------	------	------	------	------	-------	--------




Sum of corrected areas: 6689239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
Data File : VU054152.D
Acq On : 11 May 2023 11:05
Operator : JC/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK095

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

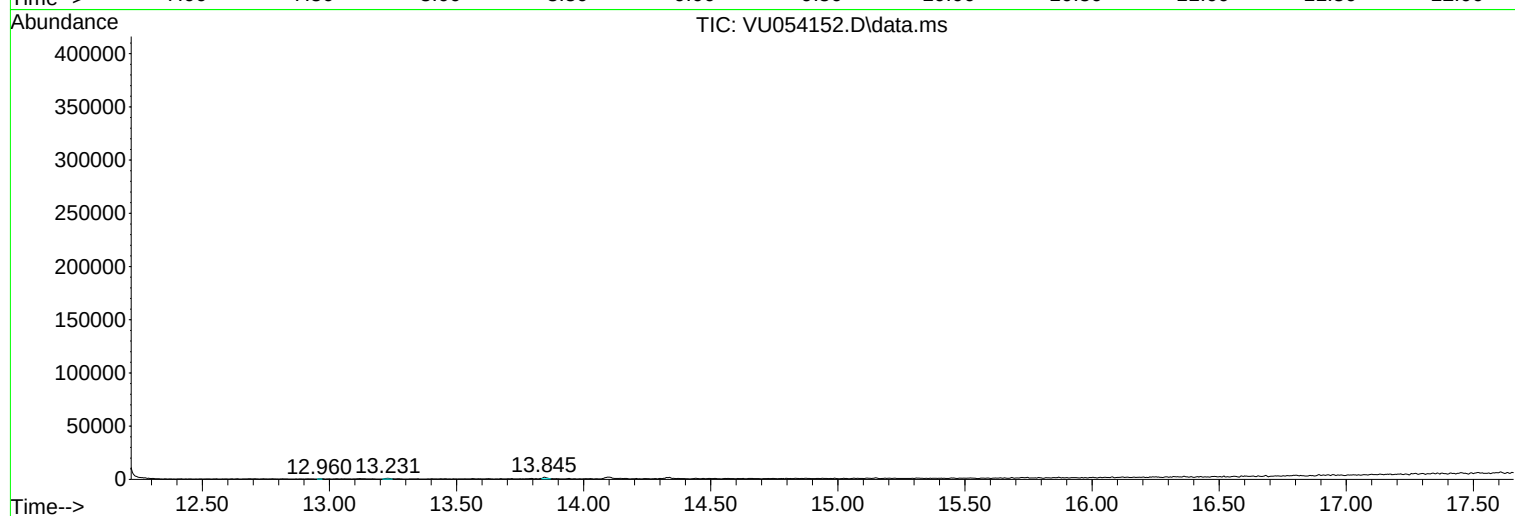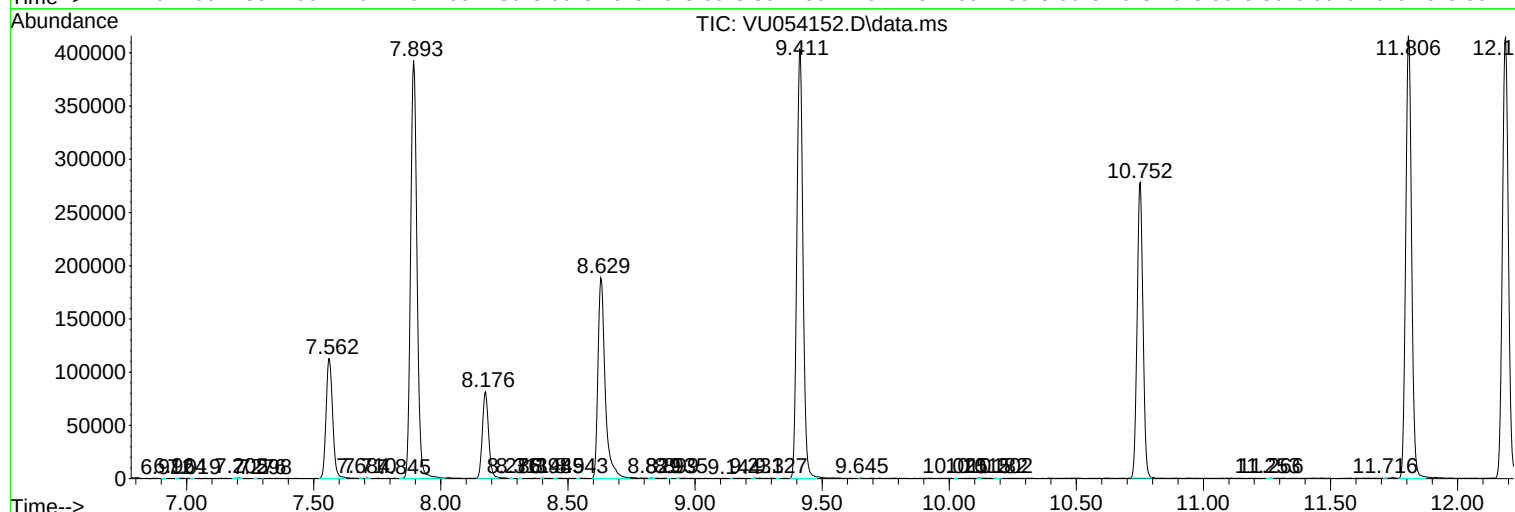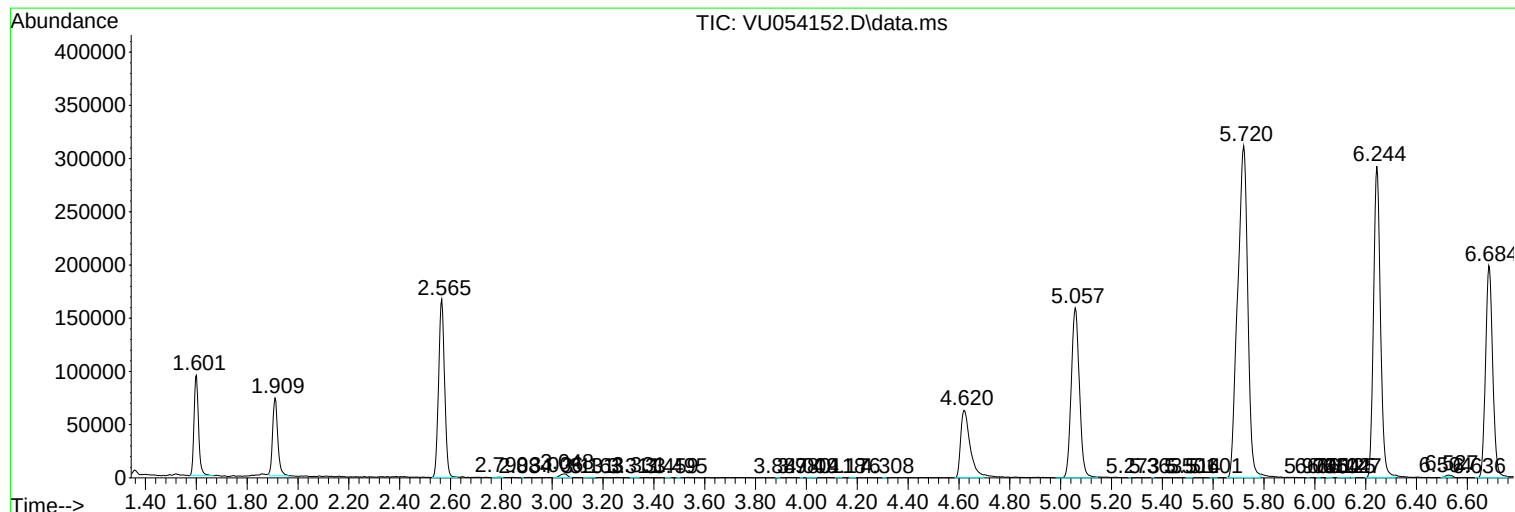

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
Data File : VU054152.D
Acq On : 11 May 2023 11:05
Operator : JC/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK095

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
Data File : VU054152.D
Acq On : 11 May 2023 11:05
Operator : JC/MD
Sample : VU0511WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK095

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------